

HUMAN ADIPONECTIN (TOTAL) ELISA KIT

FOR THE QUANTITATIVE DETERMINATION OF HUMAN ADIPONECTIN CONCENTRATIONS IN CELL CULTURE SUPERNATES, PLASMA AND SERUM



FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

PURCHASE INFORMATION:

| ELISA NAME | HUMAN ADIPONECTIN ELISA |
|-----------------------|---|
| Catalog No. | SK00010-01 |
| Lot No. | |
| Formulation | 96 T |
| Standard Range | 62.5-4000 pg/ml |
| Sensitivity | 31 pg/ml |
| Sample Volume | 100 µl |
| Sample Dilution | 2500 (Optimal dilutions should be determined by each laboratory for each application) |
| Sample Type | serum, plasma, cell culture supernates |
| Specificity | Human ADIPONECTIN only |
| Intra-assay Precision | 4-8% |
| Inter-assay Precision | 8-12% |
| Storage | 2-8°C |

ORDER CONTACT:

2348 WALSH AVE., SUITE C
SANTA CLARA, CA 95051
USA

TEL: (408) 982 0300

EMAIL:

SALES@AVISCERABIOSCIENCE.COM

WEBSITE:

WWW.AVISCERABIOSCIENCE.COM

INTRODUCTION

Human Adiponectin (Total) immunoassay is a 3.5 - 4.5 hour solid phase ELISA designed to measure total (low, middle, and high molecular weight) human Adiponectin in cell culture supernates, serum, and EDTA plasma. It contains recombinant human Adiponectin and antibodies raised against this protein. It has been shown to accurately quantify recombinant human Adiponectin. Results obtained with naturally occurring Adiponectin samples showed linear curves that were parallel to the standard curves obtained using the kit standards. These results indicate that the immunoassay kit can be used to determine relative mass values for natural human Adiponectin.

PRINCIPLE OF THE ASSAY

This assay employs the quantitative sandwich enzyme immunoassay technique. A monoclonal antibody specific for Adiponectin has been pre-coated onto a microplate. Standards and samples are pipetted into the wells and any Adiponectin present is bound by the immobilized antibody. After washing away any unbound substances, a biotinylated monoclonal antibody specific for Adiponectin is added to the wells. Following a wash to remove any unbound antibody-biotin reagent, HRP link Streptavidin is added to the wells. After washing away any unbound enzyme, a substrate solution is added to the wells and color develops in proportion to the amount of Adiponectin bound in the initial step. The color development is stopped and the intensity of the color is measured.

LIMITATIONS OF THE PROCEDURE

_ FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

_ The kit should not be used beyond the expiration date on the kit label.

_ Do not mix or substitute reagents with those from other lots or sources.

_ It is important that the Dilution Buffer selected for the standard curve be consistent with the samples being assayed.

_ If samples generate values higher than the highest standard, dilute the samples with Dilution Buffer and repeat the assay.

_ Any variation in standard diluent, operator, pipetting technique, washing technique, incubation time or temperature, and kit age can cause variation in binding.

_ This assay is designed to eliminate interference by soluble receptors, binding proteins, and other factors present in biological samples. Until all factors have been tested in the immunoassay, the possibility of interference cannot be excluded.

MATERIALS PROVIDED

| DESCRIPTION | CODE | QUANTITY |
|---|------------------|------------------|
| Adiponectin Microplate - 96 well polystyrene microplate (12 strips of 8 wells) coated with a monoclonal purified IgG against human Adiponectin. | 010-01-01 | 1 plate |
| Adiponectin Standard – 2000 pg/vial of recombinant human Adiponectin in a buffered protein base with preservatives; lyophilized. | 010-01-02 | 2 vials |
| Detection Antibody Concentrate – 105 µL/vial, 100-fold concentrated of biotinylated monoclonal purified IgG against human Adiponectin with preservatives; lyophilized. | 010-01-03 | 1 vial |
| Positive Control – one vial of recombinant human Adiponectin, lyophilized | 010-01-04 | 1 vial |
| Streptavidin-HRP Conjugate - 60 µl/vial, 200-fold concentrated solution of Streptavidin conjugate to HRP with preservatives | SAHRP | 1 vial |
| Dilution Buffer - 60mL of buffered protein based solution with preservatives | DB01 | 2 bottles |
| Wash Buffer - 50 mL of 10-fold concentrated buffered surfactant, with preservative. | WB01 | 1 bottle |
| TMB Substrate Solution - 11 mL of TMB substrate solution | TMB01 | 1 bottle |
| Stop Solution - 11mL of 0.5M HCl | S-STOP | 1 bottle |
| Plate Sealer | EAPS | 1 piece |
| Plastic Pouch | P01 | 1 piece |

STORAGE

Unopened Kit: Store at 2 - 8° C for up to 12 months. For longer storage, unopened Standard, Positive Control and Detection Antibody Concentrate should

be stored at -20°C or -70°C. Do not use kit past expiration date.

Opened / Reconstituted Reagents: Reconstituted Standard and Detection Antibody Concentrate Solution SHOULD BE STORED at -20°C or -70°C for up to one month.

Streptavidin-HRP Conjugate 200-fold Concentrate and other components may be stored at 2 - 8°C for up to 12 months.

Microplate Wells: Return unused wells to the plastic pouch with the desiccant pack, reseal along entire edge of zip-seal. Microplate may be stored for up to 6 months at 2 - 8°C after opening.

OTHER SUPPLIES REQUIRED

- Microplate reader capable of measuring absorbance at 450 nm, with the correction wavelength set at 540 nm or 570 nm.
- Microplate shaker (250-300rpm).
- Pipettes and pipette tips.
- Deionized or distilled water.
- Squirt bottle, manifold dispenser, or automated microplate washer.
- 100 mL and 500 mL graduated cylinders.

SAMPLE COLLECTION AND STORAGE

Cell Culture Supernates - Remove particulates by centrifugation and assay immediately or aliquot and store samples at ≤-20° C. Avoid repeated freeze-thaw cycles.

Serum - Use a serum separator tube (SST) and allow samples to clot for 30 minutes before centrifugation for 15 minutes at 1000 x g. Remove serum and assay immediately or aliquot and store samples at ≤ -20° C. Avoid repeated freeze-thaw cycles.

Plasma - Collect plasma using EDTA, heparin, or citrate as an anticoagulant. Centrifuge for 15 minutes at 1000 x g within 30 minutes of collection. Assay immediately or aliquot and store samples at ≤-20° C. Avoid repeated freeze-thaw cycles.

Note: Use Aprotinin (enzyme inhibitor) (Code No.: 00700-01-25) for ALL sample collection to prevent sample degradation. 0.5 TIU per ml of sample solution.

SAMPLE PREPARATION

Serum and plasma samples may need a 2500-fold dilution. A suggested 2500-fold dilution is 10 µL sample + 490 µL Dilution Buffer. Following 10 µL 50-fold diluted sample + 490 µL Dilution Buffer.

Optimal dilutions should be determined by each laboratory for each application with a pretest. Use polypropylene test tubes.


REAGENT PREPARATION

Bring all reagents to room temperature before use.

Wash Buffer - If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved. Dilute 50 mL of Wash Buffer Concentrate into deionized or distilled water (450 mL) to prepare 500 mL of Wash Buffer.

Adiponectin Standard - Refer to vial label for reconstitution volume. Reconstitute the **Adiponectin** standard with 0.5 mL of Dilution Buffer. This reconstitution produces a stock solution of 4000 pg/mL. Allow the standard to sit for a minimum of 15 minutes with gentle agitation prior to making dilutions. Pipette 250 µL of Dilution Buffer into tubes #1 to #6. Use the stock solution to produce a dilution series (below). Mix each tube thoroughly before the next transfer. The 4000 pg/mL standard serves as the high standard. The Dilution Buffer serves as the zero standard (0 pg/mL).

| TUBE | STANDARD | DILUTION BUFFER | CONCENTRATION |
|-------|----------------|-----------------|---------------|
| stock | powder | 0.5 ml | 4000 pg/ml |
| # 1 | 250µl of stock | 250µl | 2000 pg/ml |
| # 2 | 250µl of 1 | 250µl | 1000 pg/ml |
| # 3 | 250µl of 2 | 250µl | 500 pg/ml |
| # 4 | 250µl of 3 | 250µl | 250 pg/ml |
| # 5 | 250µl of 4 | 250µl | 125 pg/ml |
| # 6 | 250µl of 5 | 250µl | 62.5 pg/ml |

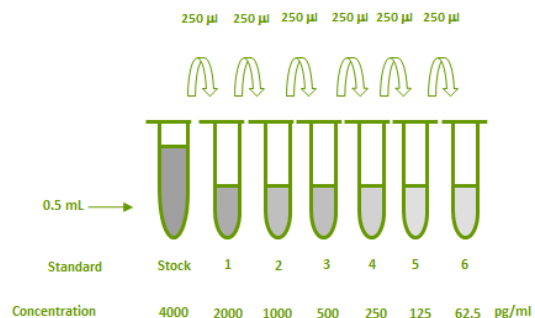

Positive Control - Reconstitute the positive control with 0.5 mL of Dilution Buffer to make positive control working solution. **Note:** Positive control working solution should be used within a few days.

Detection Antibody - Reconstitute the **Detection Antibody Concentrate** with 105 μ L of Dilution Buffer to produce a 100-fold concentrated stock solution. Pipette 10.395 mL of Dilution Buffer into a 15 mL centrifuge tube and transfer 105 μ L of 100-fold concentrated stock solution to prepare working solution.


Streptavidin-HRP Conjugate - Pipette 11.94 mL of Dilution Buffer into a 15 mL centrifuge tube and transfer 60 μ L of 200-fold concentrated stock solution to prepare working solution. **Note:** Working solution of streptavidin-HRP conjugate should be used within a few days.

ASSAY PROCEDURE

Bring all reagents and samples to room temperature before use. It is recommended that blank, standards, samples and positive control be assayed in duplicates.

1. Prepare all reagents and working standards as directed in the previous sections.
2. Remove excess micro-plate strips from the plate frame, return them to the plastic pouch with the desiccant pack, reseal.
3. Add 50 μ L of Dilution Buffer to all wells that will be used.
- 3a. Add 50 μ L of Dilution Buffer to Blank wells (B2, B3).
4. Add 50 μ L of Standard (C2, C3 to G2, G3 and F4, F5 to G4, G5), sample, or positive control (E4, E5) per well. Cover with plate sealer. Incubate for 2 hours on micro-plate shaker at room temperature. A plate layout is provided to record standards and samples assayed.
5. Aspirate each well and wash, repeating the process three times for a total of four washes. Wash by filling each well with Wash Buffer (300 μ L) using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.

6. Add 100 μ L of Detection Antibody working solution to each well. Cover with plate sealer. Incubate for 2 hours on micro-plate shaker at room temperature.
7. Repeat the aspiration/wash as in step 5.
8. Add 100 μ L of Streptavidin-HRP Conjugate working solution to each well. Incubate for 60 minutes on micro-plate shaker at room temperature. **Protect from light.**
9. Repeat the aspiration/wash as in step 5.
10. Add 100 μ L of Substrate Solution to each well. Incubate for 3-7 minutes at room temperature. **Protect from light.**
11. Add 100 μ L of Stop Solution to each well. The color in the wells should change from blue to yellow. If the color in the wells is green, or if the color change does not appear uniform, gently tap the plate to ensure thorough mixing.
12. Determine the optical density of each well within 15 minutes, using a micro-plate reader set to 450 nm.

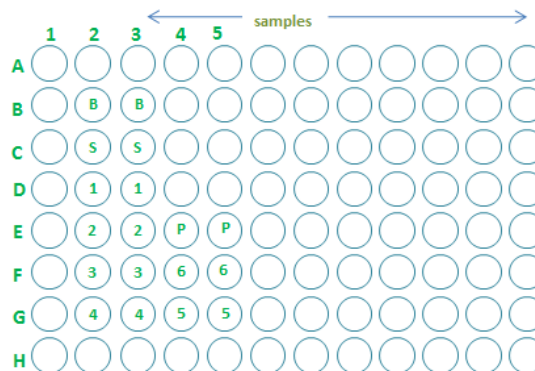

CALCULATION OF RESULTS

Average the duplicate readings for each standard, positive control, and sample and subtract the average zero standard optical density. Create a standard curve by reducing the data using computer software capable of generating a log-log curve fit. As an alternative, construct a standard curve by plotting the mean absorbance for each standard on the y-axis against the concentration on the x-axis and draw a best fit curve through the points on the graph. The data may be linearized by plotting the log of the Adiponectin concentrations versus the log of the O.D. and the best fit line can be determined by regression analysis. This procedure will produce an adequate but less precise fit of the data.

If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

TYPICAL DATA

This standard curve is for demonstration only. A standard curve should be generated for each set of samples assayed.

| STANDARD (PG/ML) | CORRECTED (450NM) |
|------------------|-------------------|
| Blank | 0 (0.081) |
| 62.5 | 0.072 |
| 125 | 0.135 |
| 250 | 0.267 |
| 500 | 0.514 |
| 1000 | 1.054 |
| 2000 | 1.825 |
| 4000 | 2.979 |

CALIBRATION

This immunoassay is calibrated against a highly purified NS0-expressed recombinant human Adiponectin.

SENSITIVITY

Twenty-five assays were evaluated and the minimum detectable dose (MDD) of Adiponectin was 31 pg/mL.

SPECIFICITY

| PROTEINS | CROSS-REACTIVITY |
|-------------------|------------------|
| Human Adiponectin | 100% |
| Mouse Adiponectin | 0 |

SUMMARY OF ASSAY PROCEDURE

| PREPARE REAGENTS, SAMPLES AND STANDARDS |
|--|
| ↓ |
| Add 50 µl of Dilution Buffer to all wells that will be used |
| ↓ |
| Add 50 µl of standard, samples, positive control to each well. Incubate for 2 hours at RT. |
| ↓ |
| Aspirate and wash 4 times. |
| ↓ |
| Add 100 µl Detection Antibody working solution to each well. Incubate for 2 hours on the plate shaker at RT. |
| ↓ |
| Aspirate and wash 4 times. |
| ↓ |
| Add 100 µl Streptavidin-HRP conjugate working solution to each well. Incubate 60 min on plate shaker at RT. Protect from light. |
| ↓ |
| Aspirate and wash 4 times. |
| ↓ |
| Add 100 µl Substrate Solution to each well. Incubate 3-7 min on the bench top. Protect from light. |
| ↓ |
| Add 100 µl Stop Solution to each well. Read 450nm within 15 min |