

MYONECTIN / CTRP15 (MOUSE, RAT, HUMAN) ELISA KIT

FOR THE QUANTITATIVE DETERMINATION OF
MYONECTIN/ CTRP15 CONCENTRATIONS IN
MOUSE,RAT AND HUMAN SERUM AND EDTA
PLASMA



ALWAYS REFER TO LOT SPECIFIC PROTOCOL
PROVIDED WITH EACH KIT FOR
INSTRUCTIONS. PROTOCOL MUST BE
READ BEFORE USING THIS PRODUCT.

FOR RESEARCH USE ONLY. NOT FOR USE IN
DIAGNOSTIC PROCEDURES.

PRODUCT INFORMATION:

ELISA NAME	MYONECTIN / CTRP 15 (MOUSE, RAT, HUMAN) ELISA KIT
Catalog No.	SK00393-10
Lot No.	
Formulation	96 T
Standard range	8-5000 ng/mL
Dynamic range	8 - 2000 ng/mL
Sensitivity	1 ng/mL
Sample Volume	50 µl per well
Dilution Factor	4 (Optimal dilutions should be determined by each laboratory for each application)
Sample Type	Serum, EDTA Plasma
Specificity	Mouse, Rat, Human
Calibration	Mouse Myonectin /CTRP15
Intra-assay Precision	6 – 8%
Inter-assay Precision	12 – 14%
Storage	2 – 8° C
This kit contains sufficient materials to run 35 samples duplicated provided that assay is run according to protocol.	

ORDER CONTACT:

AVISCIERA BIOSCIENCE, INC.
2348 Walsh Ave., Suite C
Santa Clara, CA 95051
USA

Tel: (408) 982 0300

Fax: (408) 982 0301

Email: Sales@AvisceraBioscience.com

Info@AvisceraBioscience.com

www.AvisceraBioscience.com

DESCRIPTION

Myonectin / CTRP15 (Mouse, Rat, Human) ELISA Kit contains the necessary components required for the quantitative measurement of recombinant and/or natural mouse myonectin/CTRP15 from serum and plasma in a competitive enzyme immunoassay technique format.

This immunoassay contains recombinant mouse myonectin/CTRP15 and antibodies raised against this protein. Results from this immunoassay have shown to accurately quantify recombinant and natural mouse myonectin /CTRP15 samples. The data also indicated that rat and human serum or plasma samples were competitively bound to antibody that was used in this kit formulation condition. Its linear dilution curves were parallel to the standard curves obtained using the ELISA standard. That means rat serum and plasma samples cross-react with myonectin /CTRP15 (Mouse) ELISA kit.

ASSAY OVERVIEW

Myonectin /CTRP15 (Mouse, Rat, Human) ELISA employs the quantitatively competitive enzyme immunoassay technique in which myonectin present in samples compete with a fixed amount of biotinylated myonectin for sites on an antibody specific against myonectin. Following a wash to remove any unbound standard, positive control, samples, antibody and biotin conjugate, a Streptavidin conjugated to horseradish-peroxidase (HRP) is added to the wells. After washing away any unbound enzyme, a substrate solution is added to the wells. The enzyme reaction yields a blue product that turns yellow when Stop Solution is added. The intensity of the color measured is in inverse proportion to the amount of myonectin bound in the initial step. The sample values are then read off the standard curve.

PROCEDURAL LIMITATIONS

_FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

_This ELISA kit should not be used beyond the expiration date on the kit label.

_Do not mix reagents with those from other lots or sources.

_It is important that the Dilution Buffer selected for the standard curve be consistent with the samples being assayed.

_Each laboratory must determine the optimal dilution factors for the samples being assayed with a pretest. If samples generate values that are not within the dynamic range of the standard curve, further concentrate or dilute the samples as required with Dilution Buffer and repeat the assay.

_Any modifications in buffers, pipetting technique, washing technique, incubation time or temperature, as well as kit age can cause a change in signal.

_Not all interfering factors have been tested in the immunoassay, therefore the possibility of interference cannot be excluded.

COMPONENTS PROVIDED

Description	Code	Quantity
R-Microplate - 96 well microplate pre-coated with polyclonal anti rabbit IgG Fc purified IgG.	RM01	1 plate
Myonectin Standard – 5 µg/vial of recombinant mouse myonectin in a buffered protein base with preservative; lyophilized.	393-10-01	1 vial
Biotin Solution Concentrate - 600 µL/vial, 10-fold concentrate of mouse myonectin biotinylated with preservative; lyophilized.	393-10-02	1 vial
Myonectin Antibody Concentrate – 600 µl/vial, 10-fold concentrate of polyclonal purified IgG against mouse myonectin with preservative; lyophilized.	393-10-03	1 vial
Positive Control – one vial of recombinant mouse myonectin; lyophilized (optional).	393-10-04	1 vial
Streptavidin-HRP Conjugate - 120 µl/vial, 100-fold concentrated solution of Streptavidin conjugate to HRP.	SAHRP	1 vial
Dilution Buffer – 60 mL of buffered protein based solution with preservative.	DB18	1 bottle
HRP Diluent Solution - 12 mL of buffered protein based solution with preservative.	DB06	1 bottle
Wash Buffer - 50 mL of 10-fold concentrated buffered surfactant, with preservative.	WB01	1 bottle

Substrate Solution - 11 mL of substrate solution.	SS01	1 bottle
Stop Solution - 11 mL of 0.5M HCl.	S-STOP	1 bottle
Plate Sealer	EAPS	1 piece
Plastic Pouch	P01	1 piece

STORAGE

Unopened Kit: Store at 2 - 8° C for up to 6 months. For longer storage, unopened Standard, Positive Control, Antibody Concentrate and Biotin Solution Concentrate should be stored at -20° C or -70° C. Do not use kit past expiration date.

Opened / Reconstituted Reagents: Reconstituted Standard (stock), Antibody concentrated solution and Biotin concentrated solution SHOULD BE STORED at -20° C or -70° C for up to one month. Reconstituted Biotin concentrated solution (350 µL) CAN NOT BE STORED at 2 - 8° C. Streptavidin-HRP Conjugate 100-fold concentrated solution (**protect from light**) and other components may be stored at 2 - 8° C for up to 6 months.

Microplate Wells: Return unused wells to the plastic pouch with the desiccant pack. Microplate may be stored for up to 6 months at 2 - 8° C.

ADDITIONAL MATERIALS REQUIRED

- Microplate reader capable of absorbance measurement at 450 nm.
- Microplate shaker (250 – 300 rpm).
- Microplate washer or manifold dispenser.
- 100 mL and 500 mL graduated cylinders.
- Multi-channel Pipette, Pipettes and pipette tips.
- Deionized or distilled water.

PRECAUTION

This kit should be handled by those persons who have been trained in and can follow the principles of good laboratory practice. Wear protective clothing such as laboratory overalls, safety glasses and gloves. Care should be taken while handling solutions in this kit to avoid contact with skin or eyes, especially with the stop solution because it contains diluted hydrochloric acid. Wash immediately with water in case of contact on skin or eyes.

SAMPLE COLLECTION AND STORAGE

Serum - Use a serum separator tube (SST) and allow samples to clot for 30 minutes before centrifugation

for 15 minutes at 1000 x g. Remove serum and assay immediately or aliquot and store samples at ≤ -20° C. Avoid repeated freeze-thaw cycles.

Plasma - Collect plasma using EDTA as an anticoagulant. Centrifuge for 15 minutes at 1000 x g within 30 minutes of collection. Assay immediately or aliquot and store samples at ≤ -20° C. Avoid repeated freeze-thaw cycles.

Optional: Use Aprotinin (enzyme inhibitor) for ALL sample collection to prevent sample degradation. 0.5 TIU per ml of sample solution.

SAMPLE PREPARATION

Mouse, rat and human Serum and plasma samples may need 4-fold dilution. **Optimal dilutions should be determined by each laboratory for each application.**

Use polypropylene test tubes.

REAGENT PREPARATION

Bring all reagents to room temperature before use.


Wash Buffer - If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved. Dilute 50 mL of Wash Buffer Concentrate into deionized or distilled water (450 mL) to prepare 500 mL of 1x Wash Buffer.

Myonectin Standard - Reconstitute the standard with 1 mL of Dilution Buffer. This reconstitution produces a stock solution of 5000 ng/mL. Allow the standard to sit for a minimum of 15 minutes with gentle agitation prior to making dilutions. Pipette 200 µL of Dilution Buffer into tubes #1 to #4. Use the stock solution to produce a dilution series (below). Mix each tube thoroughly before the next transfer. The **5000 ng/mL** standard serves as the high standard.

Tube	Standard	Dilution Buffer	Concentration
Stock	powder	1 ml	5000 ng/ml
# 1	50µl of stock	200µl	1000 ng/ml
# 2	50µl of 1	200µl	200 ng/ml
# 3	50µl of 2	200µl	40 ng/ml
# 4	50µl of 3	200µl	8 ng/ml

Positive Control - Reconstitute the Positive Control with 1.0 mL of Dilution Buffer. **Note:** Positive

Control could be reused within a few days if stored at -20°C or -70°C .

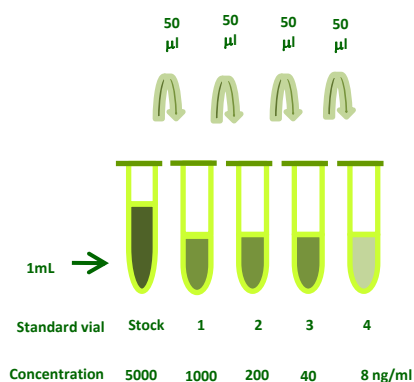

Myonectin Antibody Concentrate - Reconstitute the Myonectin Antibody Concentrate with 600 μL of Dilution Buffer to produce a 10-fold concentrated stock solution. Transfer it to 5.4 mL of Dilution Buffer to prepare **1x Antibody Solution**.

Biotin Solution Concentrate - Reconstitute the Biotin Solution Concentrate with 600 μL of Dilution Buffer to make 10-fold concentrated stock solution. Transfer it to 5.4 mL of Dilution Buffer to prepare **1x Biotin Solution**.

Streptavidin-HRP Conjugate - Transfer 120 μL of 100-fold concentrated stock solution to 11.88 mL of **HRP Diluent Solution (DB06)** to prepare working solution. **Note:** 1x working solution of Streptavidin-HRP Conjugate should be used within a few days (**protect from light**).

ELISA PROTOCOL

Bring all reagents and samples to room temperature before the start of the assay. Blank, standard dilutions, positive control and samples should be assayed in duplicate. ELISA Protocol may need further optimization.

1. Prepare all reagents and working standards as directed in the previous sections.
2. Remove excess microplate strips from the plate frame, return them to the plastic pouch with the desiccant pack.
3. Leave two wells as Blank. **DO NOT ADD ANY ANTIBODY OR BIOTIN SOLUTION INTO BLANK WELLS.**

4. Set two wells as Total Binding. Add 50 μL per well of **Dilution Buffer**.
5. Add 50 μL per well of **Standard dilutions** from #4 to #S (reverse order of serial dilution) to the appropriate wells. Add 50 μL per well of **Positive Control** into another wells. Add 50 μL per well of **samples** into other wells.
6. Add 50 μL per well of **1x Antibody Solution** into total binding, standard, positive control and sample wells. Cover with plate sealer and incubate on microplate shaker (250 - 300rpm) at room temperature for 2 hours. **Note: DO NOT ASPIRATE AND WASH PLATE. PROCEED IMMEDIATELY TO THE NEXT STEP.**
7. Add 50 μL per well of **1x Biotin Solution** into total binding, standard, positive control and sample wells. Cover with plate sealer and incubate on microplate shaker at room temperature for 2 hours. **Note: DO NOT ADD Biotin Solution to Blank wells.**
8. Aspirate wells and wash 4 times with 300 μL of **1x Wash Buffer**. Blot plate on absorbent paper to remove any residual buffer.
9. Add 100 μL of **Streptavidin-HRP Conjugate working solution** to each well, including the blanks. Incubate on microplate shaker for 40 min at room temperature. **Protect from light.**
10. Aspirate and wash as step 8.
11. Add 100 μL of **Substrate Solution** to each well. Incubate for 3-4 minutes on microplate shaker at room temperature. **Protect from light.**
12. Add 100 μL of **Stop Solution** to each well. The color in the wells should change from blue to yellow. It is recommended to add the stop solution when the total Binding or the lowest standard has developed a dark blue color.
13. Determine the optical density of each well within 15 minutes. Set the microplate reader to 450 nm.

CALCULATION OF RESULTS

Average the duplicate readings for each standard, positive control and samples, and subtract the average blank optical density. It is recommended to use software capable of generating a four parameter logistic (4-PL) curve-fit. The standard curve shows

relationship between standard concentrations and corresponding O.D absorbance. If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

TYPICAL DATA

This standard curve is provided for demonstration only. A standard curve should be generated for each set of samples assayed.

Well	OD450 reading	Standard (ng/mL)
Blank	0.057	
Total Binding	2.048	0
Standard 4	1.810	8
Standard 3	1.632	40
Standard 2	0.821	200
Standard 1	0.350	1000
Standard S	0.098	5000

SPECIFICITY

Proteins	Cross-reactivity
Mouse CTRP15	100%
Mouse CTRP13	0
Mouse CTRP12	0
Mouse CTRP9	0
Mouse CTRP1	0
Mouse Betatrophin	0
Human/Mouse Irisin	0
Mouse Meteorin Like	0
Mouse Adiponectin	0
Rat Adiponectin	0
Mouse Leptin	0

SUMMARY OF ASSAY PROCEDURE

PREPARE REAGENTS, SAMPLES AND STANDARDS
↓
Add 50 µL of standard dilutions, samples, or positive control to the wells. Add 50 µL of 1x Antibody solution to each well. Incubate 2 hours on the plate shaker at RT. Do not wash or aspirate. Proceed to next step.
↓
Add 50 µL 1x Biotin Solution to each well. Incubate 2 hours on the plate shaker at RT.
↓
Aspirate and wash 4 times.
↓
Add 100 µL Streptavidin-HRP conjugate working solution to all wells, including blanks. Incubate 1 hour on the plate shaker at RT. Protect from light.
↓
Aspirate and wash 4 times.
↓
Add 100 µL Substrate Solution to each well. Incubate 3-10 min on the plate shaker at RT. Protect from light.
↓
Add 100 µL Stop Solution to each well. Read 450nm within 15 min.