

# HIGH SENSITIVITY SOLUBLE CSF1R/CD115 HUMAN ELISA KIT

FOR THE QUANTITATIVE DETERMINATION OF  
HUMAN CSF1R CONCENTRATIONS IN PLASMA AND  
SERUM



ALWAYS REFER TO LOT SPECIFIC  
PROTOCOL PROVIDED WITH EACH KIT FOR  
INSTRUCTIONS. PROTOCOL MUST BE  
READ AND CHECK ALL ITEMS OF EACH KIT  
BEFORE USING THIS PRODUCT.

FOR RESEARCH USE ONLY. NOT FOR USE IN  
DIAGNOSTIC PROCEDURES.

## PRODUCT INFORMATION:

**THIS KIT IS FOR ONE TIME USE ONLY.**

ELISA NAME	HIGH SENSITIVITY SOLUBLE CSF1R HUMAN ELISA KIT
Catalog No.	SK00144-01
Lot No.	
Formulation	96 T
Standard range	19.5~ 1250 pg/mL
Sensitivity	10 pg/mL
Sample Volume	100 µL
Dilution Factor	400 ~ 800 (Optimal dilutions should be determined by each laboratory for each application with a pretest.)
Sample Type	Serum, plasma
Specificity	Human Soluble CSF1R
Calibration	Human Soluble CSF1R Recombinant (HEK293 derived)
Intra-assay Precision	4 - 6%
Inter-assay Precision	4 - 9%
Storage	2 – 8° C for 4 months, for longer storage more information check page 2-3
This kit contains sufficient materials to run approximately 35~40 samples duplicated provided that assay is run according to protocol.	

## Order Contact:

AVISCIERA BIOSCIENCE, INC.

2348 Walsh Ave., Suite C

Santa Clara, CA 95051

USA

Tel: (408) 982 0300

Email: [Sales@AvisceraBioscience.com](mailto:Sales@AvisceraBioscience.com)

[www.AvisceraBioscience.com](http://www.AvisceraBioscience.com)

[www.AvisceraBioscience.net](http://www.AvisceraBioscience.net)

**DESCRIPTION**

This High Sensitivity Soluble CSF1R Human ELISA Kit contains the necessary components required for the quantitative measurement of recombinant human sCSF1R (human cells derived) and/or natural human CSF1R from plasma, serum samples in a sandwich ELISA format.

This immunoassay contains human sCSF1R recombinant and antibodies raised against this protein. Results from this immunoassay have shown to accurately quantify bioactive recombinant and natural Human CSF1R in the samples.

**ASSAY OVERVIEW**

This assay employs the quantitative sandwich ELISA format. The plate is pre-coated with a monoclonal antibody specific for human CSF1R. The capture antibody can bind to the human CSF1R in the standard and samples. After washing the plate of any unbound substances, a biotinylated antibody against human CSF1R is added to the wells. After another washing of the plate, Streptavidin-HRP Conjugate is added. After the last wash to remove any unbound enzyme, a substrate solution (TMB) is added to the wells and color develops in direct proportion to the amount of human CSF1R bound in the standard solutions or samples. A standard curve can be established and sample values can be read off the standard curve.

**PROCEDURAL LIMITATIONS**

\_FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

\_This ELISA kit should not be used beyond the expiration date on the kit label.

\_Do not mix reagents with those from other lots or sources.

\_It is important that the Dilution Buffer selected for the standard curve be consistent with the samples being assayed.

\_Each laboratory must determine the optimal dilution factors for the samples being assayed with a pretest.

\_Any modifications in buffers, pipetting technique, washing technique, incubation time or temperature, as well as kit age can cause a change in signal.

\_Not all interfering factors have been tested in the immunoassay, therefore the possibility of interference cannot be excluded.

**COMPONENTS PROVIDED**

DESCRIPTION	CODE	QUANTITY
<b>CSF1R Microplate</b> - 96 well polystyrene microplate (12 strips of 8 wells) coated with a monoclonal antibody against human CSF1R.	<b>144-01-01</b>	<b>1 plate</b>
<b>CSF1R Standard</b> – 10 ng/vial of recombinant human CSF1R in a buffered protein base with preservative; lyophilized.	<b>144-01-02</b>	<b>1 vial</b>
<b>Detection Antibody Concentrate</b> – 1.2 mL/vial of 10-fold concentrate of biotinylated antibody against human CSF1R with preservative; lyophilized.	<b>144-01-03</b>	<b>1 vial</b>
<b>Positive Control Concentrated</b> - one vial of recombinant human CSF1R; lyophilized.	<b>144-01-04</b>	<b>1 vial</b>
<b>Streptavidin-HRP Conjugate</b> – 120 µL/vial, 100-fold concentrated solution of Streptavidin conjugate to HRP.	<b>SAHRP</b>	<b>1 vial</b>
<b>Dilution Buffer</b> - 45 mL of buffered protein based solution with preservative.	<b>DB05</b>	<b>1 bottle</b>
<b>Antibody Diluent Solution</b> - 12 mL of buffered protein based solution with preservative.	<b>DB11C</b>	<b>1 bottle</b>
<b>HRP Diluent Solution</b> - 12 mL of buffered protein based solution with preservative.	<b>DB08B</b>	<b>1 bottle</b>
<b>Wash Buffer</b> - 25 mL of 20-fold concentrated buffered surfactant, with preservative.	<b>WB01</b>	<b>1 bottle</b>
<b>TMB Substrate Solution</b> - 11 mL of TMB substrate solution.	<b>TMB01</b>	<b>1 bottle</b>
<b>Stop Solution</b> - 11 mL of 0.25M HCl solution.	<b>S-STOP</b>	<b>1 bottle</b>
<b>Plate Sealer</b>	<b>EAPS</b>	<b>1</b>
<b>Plastic Pouch</b>	<b>P01</b>	<b>1</b>

**STORAGE**

**Unopened Kit:** Store at 2 – 8° C up to 4 months. For longer storage up to 10 months, unopened Standard, Positive Control, Detection Antibody Concentrate, Dilution Buffer and HRP Diluent Solution should be stored at -20° C.

Streptavidin-HRP Conjugate and TMB Substrate Solution should be stored only at 2 ~ 8°C.

Do not use kit past expiration date.

**ADDITIONAL MATERIALS REQUIRED**

- Microplate reader capable of absorbance measurement at 450 nm.
- Microplate shaker (350 – 400 rpm).
- Microplate washer or manifold dispenser.
- 100 mL and 500 mL graduated cylinders.
- Multi-channel Pipette, Pipettes and pipette tips.
- Deionized or distilled water.

**PRECAUTION**

This kit should be handled by those persons who have been trained in and can follow the principles of good laboratory practice. Wear protective clothing such as laboratory overalls, safety glasses and gloves. Care should be taken while handling solutions in this kit to avoid contact with skin or eyes, especially with the stop solution because it contains diluted hydrochloric acid. Wash immediately with water in case of contact on skin or eyes.

**SAMPLE COLLECTION AND STORAGE**

**Serum** - Use a serum separator tube (SST) and allow samples to clot for 30 minutes before centrifugation for 15 minutes at 1000 x g. Remove serum and assay immediately or aliquot and store samples at ≤ -20° C. Avoid repeated freeze-thaw cycles.

**Plasma** – Collect plasma using EDTA, heparin, or citrate as an anticoagulant. Centrifuge at 1000 x g for 15 minutes and collect plasma. Assay samples immediately or aliquot and store at ≤ -20° C. Avoid repeated freeze-thaw cycles.

**Optional: Use Aprotinin (enzyme inhibitor) for ALL sample collection to prevent sample degradation. 0.5 TIU per ml of sample solution.**

**SAMPLE PREPARATION**

Serum or Plasma samples may require a 400 ~800-fold dilution. A suggested 100-fold dilution is 5 µl

sample + 495 µl Dilution Buffer. A suggested 400-fold dilution is 25 µl per well of 100-fold diluted sample + 75 µl per well of Dilution Buffer. A suggested 800-fold dilution is 12.5 µl per well of 100-fold diluted sample + 87.5 µl per well of Dilution Buffer.

**Optimal dilutions should be determined by each laboratory for each application with a pretest.**

**Use polypropylene test tubes.**

**REAGENT PREPARATION**

**Bring all reagents to room temperature before use.**

**Wash Buffer** - If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved. Dilute 25 mL of Wash Buffer Concentrate into deionized or distilled water (475 mL) to prepare 500 mL of 1x Wash Buffer.

**CSF1R Standard** - Reconstitute the CSF1R standard with 1.0 mL of Dilution Buffer. This reconstitution produces a stock solution of 10000 pg/mL. Allow the standard to sit for a minimum of 15 minutes with gentle agitation prior to making dilutions. Use the stock solution to produce a dilution series (below). Mix each tube thoroughly before the next transfer. The **1250 pg/mL** standard serves as the high standard. The Dilution Buffer serves as the zero standard (0 Pg/mL).

TUBE	STANDARD	DILUTION BUFFER	CONCENTRATION
stock	powder	1.0ml	10000 pg/ml
# 1	100 µl of stock	700 µl	1250 pg/ml
# 2	250 µl of 1	250 µl	625 pg/ml
# 3	250 µl of 2	250 µl	312.5 pg/ml
# 4	250 µl of 3	250 µl	156.25 pg/ml
# 5	250 µl of 4	250 µl	78 pg/ml
# 6	250 µl of 5	250 µl	39 pg/ml
# 7	250 µl of 6	250 µl	19.5 pg/ml

**Positive Control** - Reconstitute the Positive Control Concentrated with 1 mL of Dilution Buffer to prepare the working solution of positive control.

**Detection Antibody** - Reconstitute the Detection Antibody Concentrate with 1.2 mL of **Antibody Diluent Solution (DB11C)** to produce a 10-fold concentrated stock solution. Pipette 9.45 mL of **Antibody Diluent Solution (DB11C)** into a 15 mL centrifuge tube and transfer 1.05 mL of 10-fold

concentrated stock solution to prepare working solution.

**Streptavidin-HRP Conjugate** - Pipette 10.89 mL of **HRP Diluent Solution (DB08B)** into a 15 mL centrifuge tube and transfer 110  $\mu$ L of 100-fold concentrated stock solution to prepare working solution (**protect from light**). The working solution of Streptavidin-HRP Conjugate should be freshly prepared and used within a few hours.

## ELISA PROTOCOL

**Bring all reagents and samples to room temperature before the start of the assay. Blank, standard dilutions, positive control and samples should be assayed in duplicate. ELISA Protocol may need further optimization.**

1. Prepare all reagents and working standards as directed in the previous sections.
2. Add 100  $\mu$ L per well of Dilution Buffer to Blank wells.
3. Add 100  $\mu$ L of standard dilutions, positive control, or samples per well. Cover with the plate sealer. Incubate for **2 hours** on microplate shaker at room temperature.
4. Aspirate each well and wash, repeating the process three times for a total of four washes. Wash by filling each well with 1x Wash Buffer (300  $\mu$ L) using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.
5. Add 100  $\mu$ L of Detection Antibody working solution to each well. Cover with the plate sealer. Incubate for 2 hours on microplate shaker at room temperature.
6. Repeat the aspiration/wash as in step 4.
7. Add 100  $\mu$ L of Streptavidin-HRP Conjugate working solution to each well. Incubate for 60 minutes on microplate shaker at room temperature. **Protect from light.**
8. Repeat the aspiration/wash as in step 4.
9. Add 100  $\mu$ L of Substrate Solution to each well. Incubate for 10-15 minutes on microplate shaker at room temperature. **Protect from light.**
10. Add 100  $\mu$ L of Stop Solution to each well. The color in the wells should change from blue to yellow. If the color in the wells is green, or if the color

change does not appear uniform, gently tap the plate to ensure thorough mixing.

11. Determine the optical density of each well using a microplate reader set to 450 nm within 5 min.

## CALCULATION OF RESULTS

Create a standard curve by plotting the log of the known concentrations of the standard dilutions (x-axis) versus the log of its corresponding O.D. (y-axis) and draw the best fit line through the points. It is recommended to use computer software capable of generating a log-log or 4-Parameter curve fit to more accurately quantify the standard dilutions.

If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

## TYPICAL STANDARD CURVE


This standard curve is provided for demonstration only. A new standard curve with specific lot should be generated for each set of samples assayed.

STANDARD (PG/ML)	AVERAGE OD450NM (CORRECTED)
Blank	0 (0.085)
19.5	0.048
39	0.089
78	0.175
156	0.339
312.5	0.646
625	1.209
1250	2.295

Lot No.:

Positive Control:

Log-log standard curve:

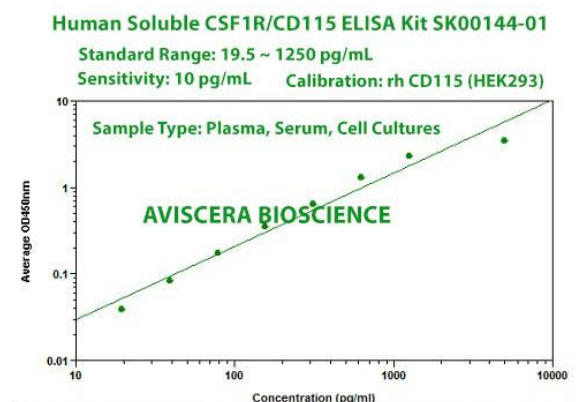

## SPECIFICITY

PROTEINS	CROSS-REACTIVITY
Human CSF1R (HEK293 derived)	100%
Mouse CSF1R (HEK293 derived)	0
Human CSF (HEK293 derived)	0

The research samples were diluted by Dilution Buffer DB05. Its recovery was assayed by Human sCSF1R/CD115 ELISA Kit SK00144-01

SAMPLE TYPE	DILUTION FACTOR	ASSAYED (PG/ML)	FINAL (NG/ML)	RECOVERY (%)
Human Plasma	400 X	3735.093	1494.037	100
Human Plasma	800 X	1987.233	1589.79	106
Human Plasma	1600 X	924.341	1478.95	99
Human Plasma	3200 X	432.591	1384.291	92.7

## SUMMARY OF ASSAY PROCEDURE

PREPARE REAGENTS, SAMPLES AND STANDARDS
↓
Add 100 µl of standard dilutions, samples, or positive control to each well. Incubate <b>2 hours</b> on the plate shaker at RT.
↓
Aspirate and wash 4 times.
↓
Add 100 µl Detection Antibody working solution to each well. Incubate 2 hours on the plate shaker at RT.
↓
Aspirate and wash 4 times.
↓
Add 100 µl Streptavidin HRP conjugate working solution to each well. Incubate 60 min on the plate shaker at RT. <b>Protect from light.</b>
↓
Aspirate and wash 4 times.
↓
Add 100 µl Substrate Solution to each well. Incubate 10-15 min on the plate shaker at RT. <b>Protect from light.</b>
↓
Add 100 µl Stop Solution to each well. Read at 450 nm within 5 min.