

HIGH SENSITIVITY SOLUBLE CSF1R HUMAN ELISA KIT

FOR THE QUANTITATIVE DETERMINATION OF
HUMAN SOLUBLE CSF1R CONCENTRATIONS IN
PLASMA AND SERUM



ALWAYS REFER TO LOT SPECIFIC
PROTOCOL PROVIDED WITH EACH KIT FOR
INSTRUCTIONS. PROTOCOL MUST BE
READ AND CHECK ALL ITEMS OF EACH KIT
BEFORE USING THIS PRODUCT.

FOR RESEARCH USE ONLY. NOT FOR USE IN
DIAGNOSTIC PROCEDURES.

PRODUCT INFORMATION:

THIS KIT IS FOR ONE TIME USE ONLY.

ELISA NAME	HIGH SENSITIVITY SOLUBLE CSF1R HUMAN ELISA KIT
Catalog No.	SK00144-06
Lot No.	20114803
Formulation	96 T
Standard range	10 ~ 640 pg/mL
Sensitivity	2 pg/mL
Sample Volume	100 µL
Dilution Factor	(Optimal dilutions should be determined by each laboratory for each application with a pretest.)
Sample Type	Serum, plasma
Specificity	Human Soluble CSF1R
Calibration	Human Soluble CSF1R Recombinant (HEK293 derived)
Intra-assay Precision	2 - 5%
Inter-assay Precision	4 - 8%
Storage	2 – 8° C for 6 months, more information check page 2-3
This kit contains sufficient materials to run approximately 35~40 samples duplicated provided that assay is run according to protocol.	

Order Contact:

AVISCERA BIOSCIENCE, INC.

2348 Walsh Ave., Suite C

Santa Clara, CA 95051

USA

Tel: (408) 982 0300

Email: Sales@AvisceraBioscience.com

www.AvisceraBioscience.com

www.AvisceraBioscience.net

DESCRIPTION

This High Sensitivity Soluble CSF1R Human ELISA Kit contains the necessary components required for the quantitative measurement of recombinant human sCSF1R (human cells derived) and/or natural human CSF1R from plasma, serum samples in a sandwich ELISA format.

This immunoassay contains human sCSF1R recombinant and antibodies raised against this protein. Results from this immunoassay have shown to accurately quantify bioactive recombinant and natural Human CSF1R in the samples.

ASSAY OVERVIEW

This assay employs the quantitative sandwich ELISA format. The plate is pre-coated with a monoclonal antibody specific for human CSF1R. The capture antibody can bind to the human CSF1R in the standard and samples. After washing the plate of any unbound substances, a biotinylated monoclonal antibody against human CSF1R is added to the wells. After another washing of the plate, Streptavidin-HRP Conjugate is added. After the last wash to remove any unbound enzyme, a substrate solution (TMB) is added to the wells and color develops in direct proportion to the amount of human CSF1R bound in the standard solutions or samples. A standard curve can be established and sample values can be read off the standard curve.

PROCEDURAL LIMITATIONS

_FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

_This ELISA kit should not be used beyond the expiration date on the kit label.

_Do not mix reagents with those from other lots or sources.

_It is important that the Dilution Buffer selected for the standard curve be consistent with the samples being assayed.

_Each laboratory must determine the optimal dilution factors for the samples being assayed with a pretest.

_Any modifications in buffers, pipetting technique, washing technique, incubation time or temperature, as well as kit age can cause a change in signal.

_Not all interfering factors have been tested in the immunoassay, therefore the possibility of interference cannot be excluded.

COMPONENTS PROVIDED

DESCRIPTION	CODE	QUANTITY
CSF1R Microplate - 96 well polystyrene microplate (12 strips of 8 wells) coated with a monoclonal antibody against human CSF1R.	144-06-01	1 plate
CSF1R Standard – 40 ng/vial of recombinant human CSF1R in a buffered protein base with preservative; lyophilized.	144-06-02	1 vial
Detection Antibody Concentrate – 1.2 mL/vial of 10-fold concentrate of biotinylated antibody against human CSF1R with preservative; lyophilized.	144-06-03	1 vial
Positive Control - one vial of recombinant human CSF1R; lyophilized.	144-06-04	1 vial
Streptavidin-HRP Conjugate – 120 µL/vial, 100-fold concentrated solution of Streptavidin conjugate to HRP.	SAHRP	1 vial
Dilution Buffer - 45 mL of buffered protein based solution with preservative.	DB05	1 bottle
Antibody Diluent Solution - 12 mL of buffered protein based solution with preservative.	DB11C	1 bottle
HRP Diluent Solution - 12 mL of buffered protein based solution with preservative.	DB08B	1 bottle
Wash Buffer 20X - 25 mL of 20-fold concentrated buffered surfactant, with preservative.	WB01	1 bottle
TMB Substrate Solution - 11 mL of TMB substrate solution.	TMB01	1 bottle
Stop Solution - 11 mL of 0.25M HCl solution.	S-STOP	1 bottle
Plate Sealer	EAPS	1
Plastic Pouch	P01	1

STORAGE

Unopened Kit: Store at 2 – 8° C up to 6 months. For longer storage up to 10 months, unopened Standard, Positive Control, Detection Antibody Concentrate, Dilution Buffer and HRP Diluent Solution should be stored at -20° C.

Streptavidin-HRP Conjugate and TMB Substrate Solution should be stored only at 2 ~ 8°C.

Do not use kit past expiration date.

ADDITIONAL MATERIALS REQUIRED

- Microplate reader capable of absorbance measurement at 450 nm.
- Microplate shaker (350 – 400 rpm).
- Microplate washer or manifold dispenser.
- 100 mL and 500 mL graduated cylinders.
- Multi-channel Pipette, Pipettes and pipette tips.
- Deionized or distilled water.

PRECAUTION

This kit should be handled by those persons who have been trained in and can follow the principles of good laboratory practice. Wear protective clothing such as laboratory overalls, safety glasses and gloves. Care should be taken while handling solutions in this kit to avoid contact with skin or eyes, especially with the stop solution because it contains diluted hydrochloric acid. Wash immediately with water in case of contact on skin or eyes.

SAMPLE COLLECTION AND STORAGE

Serum - Use a serum separator tube (SST) and allow samples to clot for 30 minutes before centrifugation for 15 minutes at 1000 x g. Remove serum and assay immediately or aliquot and store samples at ≤ -20° C. Avoid repeated freeze-thaw cycles.

Plasma – Collect plasma using EDTA, heparin, or citrate as an anticoagulant. Centrifuge at 1000 x g for 15 minutes and collect plasma. Assay samples immediately or aliquot and store at ≤ -20° C. Avoid repeated freeze-thaw cycles.

Optional: Use Aprotinin (enzyme inhibitor) for ALL sample collection to prevent sample degradation. 0.5 TIU per ml of sample solution.

SAMPLE PREPARATION

Serum or Plasma samples may require a 400 fold dilution. A suggested 40-fold dilution is 5 µl sample

+ 195 µl Dilution Buffer. A suggested 400-fold dilution is 10 µl of 40-fold diluted sample per well + 90 µl Dilution Buffer per well.

Optimal dilutions should be determined by each laboratory for each application with a pretest.

Use polypropylene test tubes.


REAGENT PREPARATION

Bring all reagents to room temperature before use.

Wash Buffer - If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved. Dilute **25 mL** of Wash Buffer Concentrate 20X into deionized or distilled water (**475 mL**) to prepare 500 mL of 1x Wash Buffer.

CSF1R Standard - Reconstitute the CSF1R standard with 1.0 mL of Dilution Buffer. This reconstitution produces a stock solution of 40000 pg/mL. Allow the standard to sit for a minimum of 15 minutes with gentle agitation prior to making dilutions. Use the stock solution to produce a dilution series (below). Mix each tube thoroughly before the next transfer. The **640 pg/mL** standard serves as the high standard. The Dilution Buffer serves as the zero standard (0 pg/mL). *Optional set 1280 pg/mL as the highest standard concentration.* Store the stock solution at - 70 °C for a few days.

TUBE	STANDARD	DILUTION BUFFER	CONCENTRATION
stock	powder	1.0ml	40000 pg/ml
optional	20 µl of stock	605 µl	1280 pg/ml
# 1	10 µl of stock	615 µl	640 pg/ml
# 2	300 µl of 1	300 µl	320 pg/ml
# 3	300 µl of 2	300 µl	160 pg/ml
# 4	300 µl of 3	300 µl	80 pg/ml
# 5	300 µl of 4	300 µl	40 pg/ml
# 6	300 µl of 5	300 µl	20 pg/ml
# 7	300 µl of 6	300 µl	10 pg/ml

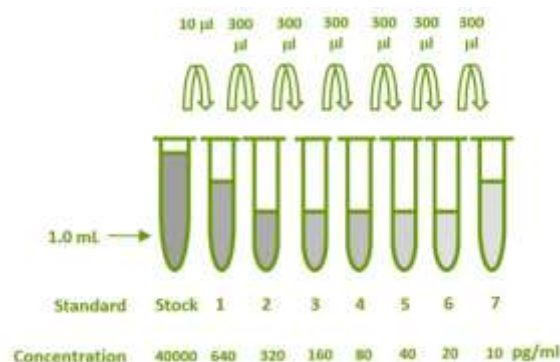

Positive Control - Reconstitute the Positive Control Concentrated with 1 mL of Dilution Buffer to prepare the working solution of positive control. Discard the working solution of positive control after use. It is for one time use only.

Detection Antibody - Reconstitute the Detection Antibody Concentrate with 1.2 mL of **Antibody Diluent Solution (DB11C)** to produce a 10-fold concentrated stock solution. For 96 well test, Freshly Pipette 9.45 mL of **Antibody Diluent Solution (DB11C)** into a 15 mL centrifuge tube and transfer 1.05 mL of 10-fold concentrated stock solution to prepare working solution. *If run a partial strip test, freshly prepare 900 µL per strip (8-wells) of working solution. Store the stock solution of 10-fold concentrated detection antibody at -20 °C for a few days.*

Streptavidin-HRP Conjugate - Freshly Pipette 10.89 mL of **HRP Diluent Solution (DB08B)** into a 15 mL centrifuge tube and transfer 110 µL of 100-fold concentrated stock solution to prepare working solution (**protect from light**). The working solution of Streptavidin-HRP Conjugate should be freshly prepared and used within 20 minutes.

If run a partial strip test, freshly prepare 900 µL per strip (8-wells) of working solution. Store the stock solution of 100-fold concentrated Streptavidin HRP at 2 -8°C for 12 months.

ELISA PROTOCOL

Bring all reagents and samples to room temperature before the start of the assay. Blank, standard dilutions, positive control and samples should be assayed in duplicate. ELISA Protocol may need further optimization.

1. Prepare all reagents and working standards as directed in the previous sections.
2. Add 100 µL per well of Dilution Buffer to Blank wells.
3. Add 100 µL of standard dilutions, positive control, or samples per well. Cover with the plate sealer. Incubate for **2 hours** on microplate shaker at room temperature.
4. Aspirate each well and wash, repeating the process three times for a total of four washes. Wash by filling each well with 1x Wash Buffer (300

µL) using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.

5. Add 100 µL of Detection Antibody working solution to each well. Cover with the plate sealer. Incubate for 90 minutes on microplate shaker at room temperature.
6. Repeat the aspiration/wash as in step 4.
7. Add 100 µL of Streptavidin-HRP Conjugate working solution to each well. Incubate for 45 minutes on microplate shaker at room temperature. **Protect from light.**
8. Repeat the aspiration/wash as in step 4.
9. Add 100 µL of Substrate Solution to each well. Incubate for 20 minutes on microplate shaker at room temperature. **Protect from light.**
10. Add 100 µL of Stop Solution to each well. The color in the wells should change from blue to yellow. If the color in the wells is green, or if the color change does not appear uniform, gently tap the plate to ensure thorough mixing.
11. Determine the optical density of each well using a microplate reader set to 450 nm within 10 min.

CALCULATION OF RESULTS

Create a standard curve by plotting the log of the known concentrations of the standard dilutions (x-axis) versus the log of its corresponding O.D. (y-axis) and draw the best fit line through the points. It is recommended to use computer software capable of generating a log-log or 4-Parameter curve fit to more accurately quantify the standard dilutions.

If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

TYPICAL STANDARD CURVE


This standard curve is provided for demonstration only. A new standard curve with specific lot should be generated for each set of samples assayed.

STANDARD (PG/ML)	AVERAGE OD450NM (CORRECTED)
Blank	0 (0.083)
10	0.029
20	0.065
40	0.119
80	0.199
160	0.385
320	0.689
640	1.273
1280 (optional)	1.999


Lot No.:

Positive Control: 150 ~ 500 pg/mL (log-log)

Standard curve by log-log fit:

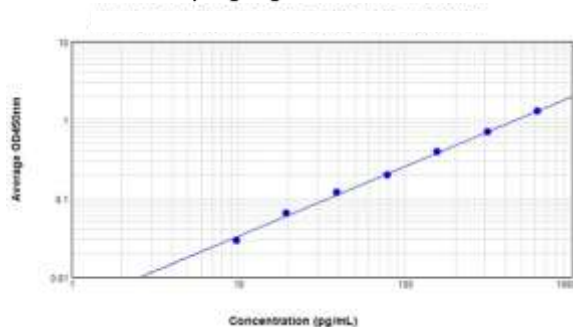


Standard curve by 4-parameter fit:

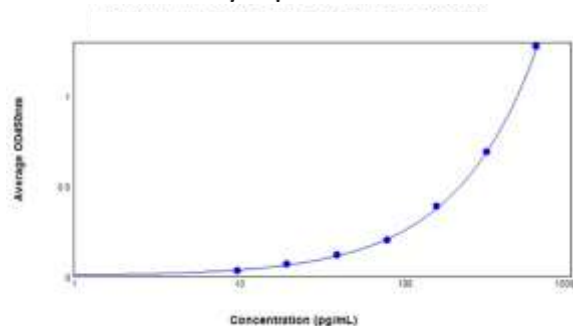

SPECIFICITY

PROTEINS	CROSS-REACTIVITY
Human CSF1R (HEK293 derived)	100%
Mouse CSF1R (HEK293 derived)	0
Human CSF (HEK293 derived)	0

Well Position

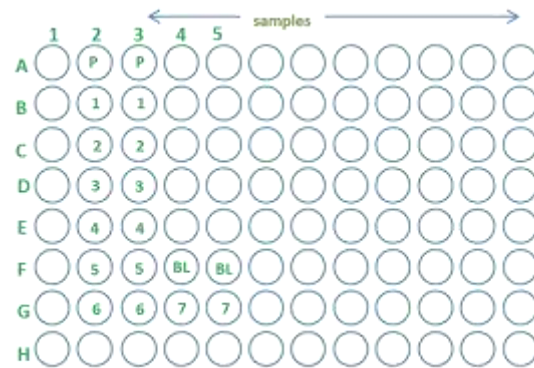

SUMMARY OF ASSAY PROCEDURE

PREPARE REAGENTS, SAMPLES AND STANDARDS
↓
Add 100 µl of standard dilutions, samples, or positive control to each well. Incubate 2 hours on the plate shaker at RT.
↓
Aspirate and wash 4 times.
↓
Add 100 µl Detection Antibody working solution to each well. Incubate 90 minutes on the plate shaker at RT.
↓
Aspirate and wash 4 times.
↓
Add 100 µl Streptavidin HRP conjugate working solution to each well. Incubate 45 min on the plate shaker at RT. Protect from light.
↓
Aspirate and wash 4 times.
↓
Add 100 µl Substrate Solution to each well. Incubate 20 min on the plate shaker at RT. Protect from light.
↓
Add 100 µl Stop Solution to each well. Read at 450 nm within 10 min.

The research samples were diluted by Dilution Buffer DB05. Its recovery was assayed by HS CSF1R ELISA Kit Sk00144-06.

Sample Type	Dilution Factor	Assayed (pg/ml)	Final (ng/ml)	Recovery (%)
EDTA Plasma	400	70.835	28.333	100
EDTA Plasma	1600	17.483	27.973	98.7
Serum	400	97.356	28.942	100
Serum	1600	23.886	28.217	98.1

New Human Endotrophin ELISA Kit SK00009-08 and SK00009-06 were developed by Aviscera Bioscience for Metabolism Syndrome and Cardiovascular Diseases Research.