

# HUMAN CTRP7 /C1QTNF7 ELISA KIT

FOR THE QUANTITATIVE DETERMINATION  
OF HUMAN CTRP7 CONCENTRATIONS IN  
SERUM AND PLASMA



ALWAYS REFER TO LOT SPECIFIC PROTOCOL  
PROVIDED WITH EACH KIT FOR  
INSTRUCTIONS. PROTOCOL MUST BE  
READ BEFORE USING THIS PRODUCT.

FOR RESEARCH USE ONLY. NOT FOR USE IN  
DIAGNOSTIC PROCEDURES.

## PRODUCT INFORMATION:

ELISA NAME	HUMAN CTRP7/C1QTNF7 ELISA KIT
Catalog No.	SK00396-09
Lot No.	
Formulation	96 T
Standard Range	1250-160000 pg/mL
Sensitivity	200 pg/mL
Sample Volume	100 µL per well
Sample Type	Serum, EDTA Plasma
Specificity	Human CTRP7
Calibration	Human CTRP7 Recombinant
Dilution Factor	<b>2-4 (Optimal dilutions should be determined by each laboratory for each application)</b>
Intra-assay Precision	6 - 8%
Inter-assay Precision	8 - 12%
Storage	2 – 8° C
This kit contains sufficient materials to run 35 samples duplicated provided that assay is run according to protocol.	

**ORDER CONTACT:**  
**AVISCERA BIOSCIENCE, INC.**  
**2348 WALSH AVE., SUITE C**  
**SANTA CLARA, CA 95051**  
**USA**  
**TEL: (408) 982 0300**  
**Email: [Info@AvisceraBioscience.com](mailto:Info@AvisceraBioscience.com)**  
**Website: [www.AvisceraBioscience.com](http://www.AvisceraBioscience.com)**

**DESCRIPTION**

This Human CTRP7 ELISA Kit contains the necessary components required for the quantitative measurement of recombinant and/or natural human CTRP7 from serum and plasma in a sandwich ELISA format.

This immunoassay contains recombinant human CTRP7 and antibodies raised against this protein. Results from this immunoassay have shown to accurately quantify recombinant and natural CTRP7 samples.

**ASSAY OVERVIEW**

This assay employs the quantitative sandwich ELISA format. The plate is pre-coated with an monoclonal antibody specific for human CTRP7. The capture antibody can bind to the human CTRP7 in the standard and samples. After washing the plate of any unbound substances, a biotinylated monoclonal antibody against human CTRP7 is added to the wells. After another washing of the plate, Streptavidin-HRP Conjugate is added. After the last wash to remove any unbound enzyme, a substrate solution (TMB) is added to the wells and color develops in direct proportion to the amount of human CTRP7 bound in the standard solutions or samples. A standard curve can be established and sample values can be read off the standard curve.

**PROCEDURAL LIMITATIONS**

\_FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

\_This ELISA kit should not be used beyond the expiration date on the kit label.

\_Do not mix reagents with those from other lots or sources.

\_It is important that the Dilution Buffer selected for the standard curve be consistent with the samples being assayed.

\_Each laboratory must determine the optimal dilution factors for the samples being assayed with a pretest. If samples generate values that are not within the dynamic range of the standard curve, further concentrate or dilute the samples as required with Dilution Buffer and repeat the assay.

\_Any modifications in buffers, pipetting technique, washing technique, incubation time or temperature, as well as kit age can cause a change in signal.

\_Not all interfering factors have been tested in the immunoassay, therefore the possibility of interference cannot be excluded.

**COMPONENTS PROVIDED**

DESCRIPTION	CODE	QUANTITY
<b>CTRP7 Microplate</b> - 96 well polystyrene microplate (12 strips of 8 wells) coated with IgG against CTRP7.	<b>396-09-01</b>	<b>1 plate</b>
<b>CTRP7 Standard</b> – 320000 pg/vial of CTRP7 in a buffered protein base with preservative; lyophilized.	<b>396-09-02</b>	<b>1 vial</b>
<b>Detection Antibody Concentrate</b> – 1.2 mL/vial, 10-fold concentrate of biotinylated IgG against CTRP7 with preservative; lyophilized.	<b>396-09-03</b>	<b>1 vial</b>
<b>Positive Control</b> - one vial of CTRP7; lyophilized.	<b>396-09-04</b>	<b>1 vial</b>
<b>Streptavidin HRP Conjugate</b> - 120 µL of 100-fold concentrated Streptavidin-HRP Conjugate.	<b>SAHRP</b>	<b>1 vial</b>
<b>Dilution Buffer</b> - 60 mL of buffered protein based solution with preservative.	<b>DB01</b>	<b>1 bottle</b>
<b>Antibody Diluent Solution</b> - 12 mL of buffered protein based solution with preservative.	<b>DB48</b>	<b>1 bottle</b>
<b>HRP Diluent Solution</b> - 12 mL of buffered protein based solution with preservative.	<b>DB06</b>	<b>1 bottle</b>
<b>Wash Buffer</b> - 50 mL of 10-fold concentrated buffered surfactant, with preservative.	<b>WB01</b>	<b>1 bottle</b>
<b>TMB Substrate Solution</b> - 11 mL of TMB substrate solution.	<b>TMB01</b>	<b>1 bottle</b>
<b>Stop Solution</b> - 11 mL of 0.5M HCl.	<b>S-STOP</b>	<b>1 bottle</b>
<b>Plate Sealer</b>	<b>EAPS</b>	<b>1 piece</b>
<b>Plastic Pouch</b>	<b>P01</b>	<b>1 piece</b>

**STORAGE**

**Unopened Kit:** Store at 2 – 8° C for up to 8 months. For longer storage, unopened Standard, Positive Control and Detection Antibody Concentrate should be stored at -20° C or -70° C. Do not use kit past expiration date.

**Opened / Reconstituted Reagents:** Reconstituted Standard (stock) solution and Detection Antibody concentrated solution SHOULD BE STORED at -20° C or -70° C for up to one month. Streptavidin-HRP Conjugate 100-fold concentrated solution and TMB Substrate Solution can be stored at 2 – 8° C for up to 8 months (**DO NOT FREEZE** and **PROTECT FROM LIGHT**). All other components may be stored at 2 – 8° C for up to 8 months.

**Microplate Wells:** Return unused strips to the plastic pouch with the desiccant pack. Microplate may be stored for up to 6 months at 2 – 8° C after opening.

### ADDITIONAL MATERIALS REQUIRED

- Microplate reader capable of absorbance measurement at 450 nm.
- Microplate shaker (250 – 300 rpm).
- Microplate washer or manifold dispenser.
- 100 mL and 500 mL graduated cylinders.
- Multi-channel Pipette, Pipettes and pipette tips.
- Deionized or distilled water.

### PRECAUTION

This kit should be handled by those persons who have been trained in and can follow the principles of good laboratory practice. Wear protective clothing such as laboratory overalls, safety glasses and gloves. Care should be taken while handling solutions in this kit to avoid contact with skin or eyes, especially with the stop solution because it contains diluted hydrochloric acid. Wash immediately with water in case of contact on skin or eyes.

### SAMPLE COLLECTION AND STORAGE

**Serum** - Use a serum separator tube (SST) and allow samples to clot for 30 minutes before centrifugation for 15 minutes at 1000 x g. Remove serum and assay immediately or aliquot and store samples at ≤ -20° C. Avoid repeated freeze-thaw cycles.

**Plasma** - Collect plasma using EDTA, heparin, or citrate as an anticoagulant. Centrifuge for 15 minutes at 1000 x g within 30 minutes of collection. Assay immediately or aliquot and store samples at ≤ -20° C. Avoid repeated freeze-thaw cycles.

**Optional: Use Aprotinin (enzyme inhibitor) (Code No.: 00700-01-25) for ALL sample collection to prevent sample degradation. 0.5 TIU per ml of sample solution.**

### SAMPLE PREPARATION

Plasma samples may require a 2-4 fold dilution. A suggested 2-fold dilution is 125 µL sample + 125 µL Dilution Buffer. A suggested 4-fold dilution is 70 µL sample + 210 µL Dilution Buffer. Plasma samples may require a 4 fold or high dilution. A suggested 4-fold dilution is 70 µL sample + 210 µL Dilution Buffer.

**Optimal dilutions should be determined by each laboratory for each application.**  
Use polypropylene test tubes.


### REAGENT PREPARATION

**Bring all reagents to room temperature before use.**

**Wash Buffer** - If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved. Dilute 50 mL of Wash Buffer Concentrate into deionized or distilled water (450 mL) to prepare 500 mL of 1x Wash Buffer.

**CTRP7 Standard** - Reconstitute the CTRP7 standard with 1 mL of Dilution Buffer. This reconstitution produces a stock solution of 320000 pg/mL. Allow the standard to sit for a minimum of 15 minutes with gentle agitation prior to making dilutions. Pipette 250 µL of the appropriate Dilution Buffer into tubes #1 to #6. Use the stock solution to produce a dilution series (below). Mix each tube thoroughly before the next transfer. The **80000 pg/mL** standard serves as the high standard. The appropriate Dilution Buffer serves as the zero standard (0 pg/mL).

TUBE	STANDARD	DILUTION BUFFER	CONCENTRATION
Stock	Powder	1000 µl	320000 pg/ml
# 1	250 µl of stock	250 µl	160000 pg/ml
# 2	250 µl of 1	250 µl	80000 pg/ml
# 3	250 µl of 2	250 µl	40000 pg/ml
# 4	250 µl of 3	250 µl	20000 pg/ml
# 5	250 µl of 4	250 µl	10000 pg/ml
# 6	250 µl of 5	250 µl	5000 pg/ml
# 7	250 µl of 6	250 µl	2500 pg/ml
# 8	250 µl of 7	250 µl	1250 pg/ml

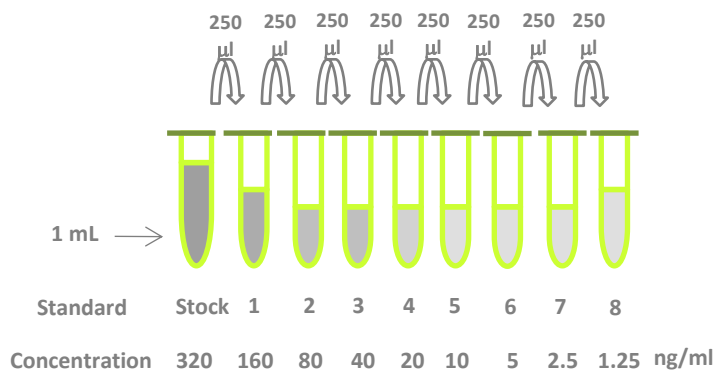

**Positive Control** – Reconstitute the Positive Control with 1 mL of Dilution Buffer to prepare working solution. **Note:** Positive Control solution could be reused within a few days if stored at  $-20^{\circ}\text{C}$  or  $-70^{\circ}\text{C}$ .

**Detection Antibody Concentrate** – Reconstitute the Detection Antibody Concentrate with 1.2 mL of Antibody Dilute Solution DB48 to produce a 10-fold concentrated stock solution. Pipette 10.8 mL of Antibody Dilute Solution DB48 into a 15 mL centrifuge tube and transfer 1.2 mL of 10-fold concentrated stock solution to prepare working solution.

**Streptavidin HRP Conjugate** – Pipette 11.88 mL of HRP Diluent Solution (DB06) into a 15 mL centrifuge tube and transfer 120  $\mu\text{L}$  of 100-fold concentrated stock solution to prepare working solution. **Note:** 1x working solution of Streptavidin-HRP Conjugate should be used within a few days (**protect from light**).

## ELISA PROTOCOL

**Bring all reagents and samples to room temperature before the start of the assay. Blank, standard dilutions, positive control and samples should be assayed in duplicate. ELISA Protocol may need further optimization.**

1. Prepare all reagents and working standards as directed in the previous sections.
2. Remove excess microplate strips from the plate frame, return them to the plastic pouch with the desiccant pack.
3. Add 100  $\mu\text{L}$  per well of Dilution Buffer to Blank wells.
4. Add 100  $\mu\text{L}$  of Standard dilutions, sample, or positive control per well. Cover with plate sealer.

Incubate for 2 hours on microplate shaker at room temperature.

5. Aspirate each well and wash, repeating the process three times for a total of four washes. Wash by filling each well with 1x Wash Buffer (300  $\mu\text{L}$ ) using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.
6. Add 100  $\mu\text{L}$  of Detection Antibody working solution to each well. Cover with plate sealer. Incubate for 2 hours on microplate shaker at room temperature.
7. Repeat the aspiration/wash as in step 5.
8. Add 100  $\mu\text{L}$  of Streptavidin-HRP working solution to each well. Cover with plate sealer. Incubate for 40 minutes on microplate shaker at room temperature. **Protect from light.**
9. Repeat the aspiration/wash as in step 5.
10. Add 100  $\mu\text{L}$  of TMB Substrate Solution to each well. Incubate for 5-9 minutes on microplate shaker at room temperature. **Protect from light.**
11. Add 100  $\mu\text{L}$  of Stop Solution to each well. The color in the wells should change from blue to yellow. If the color in the wells is green, or if the color change does not appear uniform, gently tap the plate to ensure thorough mixing.
12. Determine the optical density of each well within 15 minutes, using a microplate reader set to 450 nm.

## CALCULATION OF RESULTS

Create a standard curve by plotting the log of the known concentrations of the standard dilutions (x-axis) versus the log of its corresponding O.D. (y-axis) and draw the best fit line through the points. It is recommended to use computer software capable of generating a log-log curve fit to more accurately quantify the standard dilutions.

If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

**TYPICAL STANDARD CURVE**

This standard curve is provided for demonstration only. A new standard curve should be generated for each set of samples assayed.

STANDARD (PG/ML)	CORRECTED (450NM)
Blank	0 (0.079)
1250	0.026
2500	0.052
5000	0.112
10000	0.236
20000	0.464
40000	0.732
80000	1.273
160000	2.036

**SPECIFICITY**

PROTEINS	CROSS-REACTIVITY (%)
Human CTRP7	100
Human CTRP15	0
Human CTRP13	0
Human CTRP9	0
Human CTRP3	0
Human CTRP2	0
Human Acrp30	0

**LINEARITY**

To assess the linearity of the assay pooled research human serum samples were diluted with Dilution Buffer (DB01). The recovery of CTRP7 in human serum samples was assayed by Human CTRP7 ELISA Kit SK00396-09.

DILUTION FACTOR	ASSAYED (NG/ML)	FINAL (NG/ML)	RECOVERY (%)
1 X	over	over	
2 X	28.446	56.892	100
4 X	14.890	59.560	105

To assess the linearity of the assay pooled research human plasma samples were diluted with Dilution Buffer (DB01). The recovery of CTRP7 in human serum samples was assayed by Human CTRP7 ELISA Kit SK00396-09.

DILUTION FACTOR	ASSAYED (NG/ML)	FINAL (NG/ML)	RECOVERY (%)
1 X	18.516	18.516	100
2 X	10.850	21.700	117
4 X	5.379	21.480	116

**SUMMARY OF ASSAY PROCEDURE**

