

HIGH SENSITIVITY EOSINOPHIL CATIONIC PROTEIN (ECP) HUMAN ELISA KIT

FOR THE QUANTITATIVE DETERMINATION OF
HUMAN EOSINOPHIL CATIONIC PROTEIN (ECP)
CONCENTRATIONS IN SERUM AND EDTA
PLASMA



ALWAYS REFER TO LOT SPECIFIC
PROTOCOL PROVIDED WITH EACH KIT FOR
INSTRUCTIONS. PROTOCOL MUST BE
READ AND CHECK ALL ITEMS OF EACH KIT
BEFORE USING THIS PRODUCT.

FOR RESEARCH USE ONLY. NOT FOR USE IN
DIAGNOSTIC PROCEDURES.

PRODUCT INFORMATION:

THIS KIT IS FOR ONE TIME USE ONLY.

ELISA NAME	HIGH SENSITIVITY EOSINOPHIL CATIONIC PROTEIN (ECP) HUMAN ELISA KIT
Catalog No.	SK00128-06
Lot No.	
Formulation	96 T
Standard range	9.75 - 1250 pg/ml
Sensitivity	3 pg/ml
Sample require	100 µl
Dilution Factor	<i>Optimal dilutions should be determined by each laboratory for each application</i>
Sample Type	Serum, EDTA Plasma
Specificity	Human Eosinophil Cationic Protein (ECP)
Calibration	Human Eosinophil Cationic Protein (ECP) Rec. from HEK293 cells
Intra-assay Precision	4 - 6%
Inter-assay Precision	4 - 9%
Storage	2 - 8°C for 4 months. See page 3 for detail
This kit contains sufficient materials to run 35-40 samples duplicated provided that assay is run according to protocol.	

Order Contact:

AVISCERA BIOSCIENCE, INC.
2348 Walsh Ave., Suite C
Santa Clara, CA 95051
USA

Tel: (408) 982 0300

Email: Sales@AvisceraBioscience.com

Info@AvisceraBioscience.com

www.AvisceraBioscience.com

www.AvisceraBioscience.net

DESCRIPTION

This High Sensitivity Human Eosinophil Cationic Protein (ECP) ELISA Kit contains the necessary components required for the quantitative measurement of human ECP from serum and EDTA plasma in a sandwich ELISA format.

This immunoassay contains human Eosinophil Cationic Protein (ECP) from human cells HEK293 animal free and antibodies raised against this protein. Results from this immunoassay have shown to accurately quantify recombinant and natural ECP samples.

ASSAY OVERVIEW

This assay employs the quantitative sandwich ELISA format. The plate is pre-coated with an antibody specific for human ECP. The capture antibody can bind to the human ECP in the standard and samples. After washing the plate of any unbound substances, a biotinylated antibody against ECP is added to the wells. After another washing of the plate, Streptavidin-HRP Conjugate is added. After the last wash to remove any unbound enzyme, a substrate solution is added to the wells and color develops in direct proportion to the amount of human ECP bound in the standard solutions or samples. A standard curve can be established and sample values can be read off the standard curve.

PROCEDURAL LIMITATIONS

_FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

_This ELISA kit should not be used beyond the expiration date on the kit label.

_Do not mix reagents with those from other lots or sources.

_It is important that the Dilution Buffer selected for the standard curve be consistent with the samples being assayed.

_Each laboratory must determine the optimal dilution factors for the samples being assayed.

_Any modifications in buffers, pipetting technique, washing technique, incubation time or temperature, as well as kit age can cause a change in signal.

_Not all interfering factors have been tested in the immunoassay, therefore the possibility of interference cannot be excluded.

COMPONENTS PROVIDED

DESCRIPTION	CODE	QUANTITY
Eosinophil Cationic Protein (ECP) Microplate - 96 well polystyrene microplate coated with a purified antibody against Eosinophil Cationic Protein (ECP).	128-06-01	1 plate
Eosinophil Cationic Protein (ECP) Standard – 5 ng/vial of human Eosinophil Cationic Protein (ECP) in a buffered protein base with preservative; lyophilized.	128-06-02	1 vial
Detection Antibody – 1.2 mL/vial, 10-fold concentrate of a biotinylated antibody against Eosinophil Cationic Protein (ECP) with preservative; lyophilized.	128-06-03	1 vial
Positive Control – one vial of human Eosinophil Cationic Protein (ECP); lyophilized.	128-06-04	1 vial
Streptavidin HRP Conjugate - 120 µl/vial, 100-fold concentrated solution of Streptavidin-HRP conjugate.	SAHRP	1 vial
Dilution Buffer – 45 mL of buffered protein based solution with preservative.	DB18	1 bottle
Antibody Diluent Solution – 20 mL of buffered protein based solution with preservative.	DB18B	1 bottle
HRP Diluent Solution – 12 mL of buffered protein based solution with preservative.	DB08B	1 bottle
Wash Buffer 20X - 25 mL of 20-fold concentrated buffered surfactant, with preservative.	WB01	1 bottle
TMB Substrate Solution -11 mL of TMB substrate solution.	TMB01	1 bottle

Stop Solution - 11 mL of 0.25M HCl.	S-STOP	1 bottle
Plate Sealer	EAPS	1
Plastic Pouch	P01	1

STORAGE

Unopened Kit: Store at 2 - 8°C for up to 4 months. For longer storage up to 10 months, unopened Standard, Positive Control and Detection Antibody Concentrate, Diluent Buffer and HRP Diluent Solution should be stored at -20°C. Streptavidin HRP Conjugate and TMB Substrate Solution should be stored only at 2 ~ 8 ° C. Do not use kit past expiration date.

ADDITIONAL MATERIALS REQUIRED

- Microplate reader capable of absorbance measurement at 450 nm.
- Microplate shaker (350 – 400 rpm).
- Microplate washer or manifold dispenser.
- 100 mL and 500 mL graduated cylinders.
- Multi-channel Pipette, Pipettes and pipette tips.
- Deionized or distilled water.

PRECAUTION

This kit should be handled by those persons who have been trained in and can follow the principles of good laboratory practice. Wear protective clothing such as laboratory overalls, safety glasses and gloves. Care should be taken while handling solutions in this kit to avoid contact with skin or eyes, especially with the stop solution because it contains diluted hydrochloric acid. Wash immediately with water in case of contact on skin or eyes.

SAMPLE COLLECTION AND STORAGE

Serum - Use a serum separator tube (SST) and allow samples to clot for 30 minutes before centrifugation for 15 minutes at 1000 x g. Remove serum and assay immediately or aliquot and store samples at ≤ -20° C. Avoid repeated freeze-thaw cycles.

Plasma - Collect plasma using EDTA, heparin, or citrate as an anticoagulant. Centrifuge for 15 minutes at 1000 x g within 30 minutes of collection. Assay immediately or aliquot and store samples at ≤ -20° C. Avoid repeated freeze-thaw cycles.

SAMPLE PREPARATION

Plasma or serum samples may require 160 fold dilution.

A suggested 80 -fold dilution is 5 µL sample + 395 µL **Dilution Buffer (DB18)**. A suggested 160 -fold dilution is 50 µL per well of 80-fold diluted sample + 50 µL **Dilution Buffer (DB18)**.

Optimal dilutions should be determined by each laboratory for each application. It is very important to pretest the sample dilution before performing the final assay.

Use polypropylene test tubes.


REAGENT PREPARATION

Bring all reagents to room temperature before use.

Wash Buffer - If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved. Dilute **25 mL of Wash Buffer Concentrate 20X** into deionized or distilled water (**475 mL**) to prepare 500 mL of 1x Wash Buffer.

Eosinophil Cationic Protein (ECP) Standard - Reconstitute the **Eosinophil Cationic Protein (ECP) standard** with 1.0 mL of **Dilution Buffer DB18**. This reconstitution produces a stock solution of 5 ng/mL. Allow the standard to sit for a minimum of 15 minutes with gentle agitation prior to making dilutions. Pipette 250 µL of **Dilution Buffer (DB18)** into tubes #1 to #8. Use the stock solution (20 ng/mL) to produce a dilution series (below). Mix each tube thoroughly before the next transfer. The **1250 pg/mL** standard serves as the high standard. **The Dilution Buffer (DB18)** serves as the zero standard (0 pg/mL).

TUBE	STANDARD	DILUTION BUFFER	CONCENTRATION
stock	powder	1.0 mL	20000 pg/ml
# 1	50µl of stock	750µl	1250 pg/ml
# 2	250µl of 1	250µl	625 pg/ml
# 3	250µl of 2	250µl	312.5 pg/ml
# 4	250µl of 3	250µl	156 pg/ml
# 5	250µl of 4	250µl	78 pg/ml
# 6	250µl of 5	250µl	39 pg/ml
# 7	250µl of 6	250µl	19.5 pg/ml
# 8	250µl of 7	250µl	9.75 pg/ml

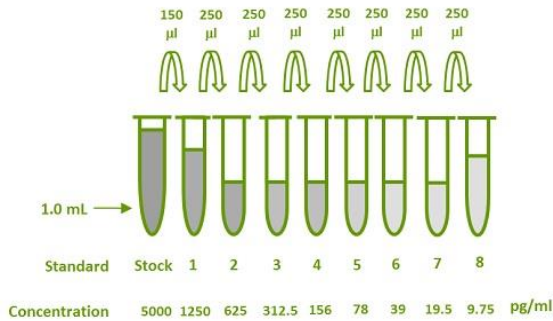

Positive Control - Reconstitute the Positive Control with 1 mL of **Dilution Buffer (DB18)** to make working solution. Discard the working solution after use. It is for one time use only.

Detection Antibody - Reconstitute the Detection Antibody Concentrate with **1.2 mL** of **Antibody Diluent Solution (DB18B)** to produce a 10-fold concentrated stock solution. For the 96 well test, freshly Transfer 1.2 mL of 10-fold concentrated stock solution to 10.8 mL of **Antibody Diluent Solution (DB18B)** to prepare working solution.

Streptavidin-HRP Conjugate - For the 96 wells test, Freshly Transfer 110 µL of 100-fold concentrated Streptavidin-HRP conjugate stock solution to 10.89 mL of **HRP Diluent Solution (DB08B)** to prepare working solution (protect from light). The 1 x working solution should be used in 10 minutes. **DO NOT FREEZE.**

ELISA PROTOCOL

Bring all reagents and samples to room temperature before the start of the assay. Blank, standard dilutions, positive control and samples should be assayed in duplicate. ELISA Protocol may need further optimization.


1. Prepare all reagents and working standards as directed in the previous sections.
2. Add 100 µL per well of Dilution Buffer (**DB18**) to Blank wells.
3. Add 100 µL of Standard solution from #8 to #1 (reverse order of serial dilution), samples, or positive control per well. Cover with plate sealer. Incubate for 2 hours on microplate shaker at room temperature.
4. Aspirate each well and wash, repeating the process three times for a total of four washes.

Wash by filling each well with 1x Wash Buffer (300 µL) using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.


5. Add 100 µL of Detection Antibody working solution to each well. Cover with plate sealer. Incubate for 2 hours on microplate shaker at room temperature.
6. Repeat the aspiration/wash as in step 4.
7. Add 100 µL of Streptavidin-HRP Conjugate working solution to each well. Incubate for 60 minutes on microplate shaker at room temperature. **Protect from light.**
8. Repeat the aspiration/wash as in step 4.
9. Add 100 µL of Substrate Solution to each well. Incubate for 12 ~ 15 minutes on microplate shaker at room temperature. **Protect from light.**
10. Add 100 µL of Stop Solution to each well. The color in the wells should change from blue to yellow. If the color in the wells is green, or if the color change does not appear uniform, gently tap the plate to ensure thorough mixing.
11. Determine the optical density of each well within 3 minutes, using a microplate reader set to 450 nm.

CALCULATION OF RESULTS

Create a standard curve by plotting the log of the known concentrations of the standard dilutions (x-axis) versus the log of its corresponding O.D. (y-axis) and draw the best fit line through the points. It is recommended to use computer software capable of generating a log-log or 4-parameter curve fit to more accurately quantify the standard dilutions. If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

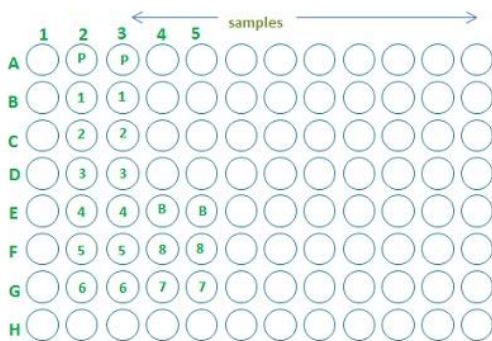

Standard curve fit by log-log:

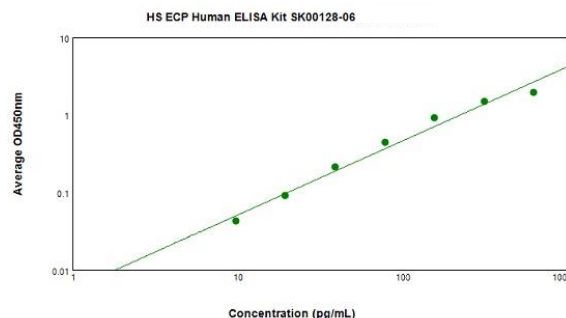

TYPICAL STANDARD CURVE

This standard curve is provided for demonstration only. A standard curve should be generated for each set of samples assayed.

STANDARD (PG/ML)	AVERAGE OD450 NM (CORRECTED*)
Blank	0 (0.119)
9.75	0.041
19.5	0.090
39.06	0.212
78.125	0.437
156.25	0.910
312.5	1.487
625	1.910
1250	2.211

- Lot No.:
- Positive Control: lot specific

SPECIFICITY

PROTEIN	CROSS-REACTIVITY (%)
Human Eosinophil Cationic Protein (ECP) from Human Eosinophils	100
Human Eosinophil Cationic Protein (ECP) Recombinant (HEK293 derived)	100
Human Eosinophil Cationic Protein (ECP); <i>E. coli</i> derived recombinant	1-2
Mouse ECP Rec (<i>E. Coli</i> derived)	0

Standard curve fit by 4-parameter:

High Sensitivity ECP (Human) ELISA Kit

Catalog No.: SK00128-06 Size: 96 T


Sensitivity: 3 pg/mL

Standard Range: 9.75 ~ 1250 pg/mL







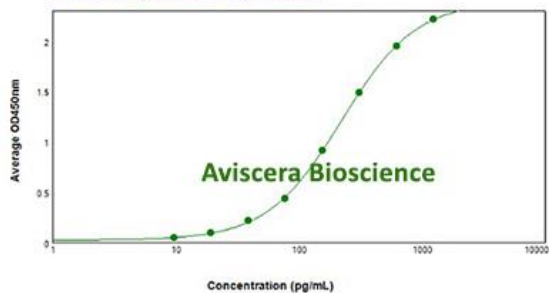

Calibration: Human ECP (HEK293)

Specificity: Human ECP

Sample Type: Serum, Plasma



SUMMARY OF ASSAY PROCEDURE

PREPARE REAGENTS, SAMPLES AND STANDARDS

Add 100 µl of standard dilutions, samples, or positive control to the well. Incubate 2 hours on plate shaker at RT.

Aspirate and wash 4 times.

Add 100 µl Detection Antibody working solution to each well. Incubate 2 hours on the plate shaker at RT.

Aspirate and wash 4 times.

Add 100 µl Streptavidin-HRP conjugate working solution to each well. Incubate 60 min on the plate shaker at RT. Protect from light.

Aspirate and wash 4 times.

Add 100 µl Substrate Solution to each well. Incubate 12 ~15 min on the plate shaker at RT. Protect from light.

Add 100 µl Stop Solution to each well. Read 450nm within 3 min.