

SOLUBLE PANCREATIC DERIVED FACTOR/FAM3B (HUMAN) ELISA KIT

FOR THE QUANTITATIVE DETERMINATION OF HUMAN PANCREATIC DERIVED FACTOR/FAM3B CONCENTRATIONS IN CELL CULTURE SUPERNATES, SERUM AND EDTA PLASMA



ALWAYS REFER TO LOT SPECIFIC PROTOCOL PROVIDED WITH EACH KIT FOR INSTRUCTIONS. PROTOCOL MUST BE READ BEFORE USING THIS PRODUCT.

FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

PURCHASE INFORMATION:

ELISA NAME	SOLUBLE PANCREATIC DERIVED FACTOR/FAM3B (HUMAN) ELISA
Catalog No.	SK00344-01
Lot No.	
Formulation	96 T
Standard Range	6.25-200 ng/mL
Sensitivity	1.5 ng/mL
Sample Volume	100 µL
Sample Type	Serum, EDTA Plasma, Cell Culture Supernates
Dilution Factor	Optimal dilutions should be determined by each laboratory for each application
Specificity	Human FAM3B
Calibration	Human FAM3B recombinant
Intra-assay Precision	4 - 6%
Inter-assay Precision	8 - 10%
Storage	2 - 8 °C
This kit contains sufficient materials to run 35 samples duplicated provided that assay is run according to protocol.	

Order Contact:
 AVISCERA BIOSCIENCE, INC.
 2348 Walsh Ave., Suite C
 Santa Clara, CA 95051
 USA
 Tel: (408) 982 0300
 Fax: (408) 982 0301
 Email: Sales@AvisceraBioscience.com
Info@AvisceraBioscience.com
www.AvisceraBioscience.com

DESCRIPTION

This Human soluble Pancreatic Derived Factor/FAM3B ELISA Kit contains the necessary components required for the quantitative measurement of recombinant and/or natural human Pancreatic Derived Factor/FAM3B from cell culture supernates, serum and plasma in a sandwich ELISA format.

This immunoassay contains recombinant human Pancreatic Derived Factor/FAM3B and antibodies raised against this protein. Results from this immunoassay have shown to accurately quantify recombinant and natural Pancreatic Derived Factor/FAM3B samples.

ASSAY OVERVIEW

This assay employs the quantitative sandwich ELISA format. The plate is pre-coated with an antibody specific for human Pancreatic Derived Factor/FAM3B. The capture antibody can bind to the human Pancreatic Derived Factor/FAM3B in the standard and samples. After washing the plate of any unbound substances, an antibody-biotin conjugate against human Pancreatic Derived Factor/FAM3B is added to the wells. After the wash to remove any unbound antibody, Streptavidin HRP conjugate is added to the wells. After the last wash to remove unbound enzyme, a substrate solution is added to the wells and color develops in direct proportion to the amount of human Pancreatic Derived Factor/FAM3B bound in the standard solutions or samples. A standard curve can be established and sample values can be read off the standard curve.

PROCEDURAL LIMITATIONS

_FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

_This ELISA kit should not be used beyond the expiration date on the kit label.

_Do not mix reagents with those from other lots or sources.

_It is important that the Dilution Buffer selected for the standard curve be consistent with the samples being assayed.

_Each laboratory must determine the optimal dilution factors for the samples being assayed with a pretest. If samples generate values that are not within the dynamic range of the standard curve, further concentrate or dilute the samples as required with Dilution Buffer and repeat the assay.

_Any modifications in buffers, pipetting technique, washing technique, incubation time or temperature, as well as kit age can cause a change in signal.

_Not all interfering factors have been tested in the immunoassay, therefore the possibility of interference cannot be excluded.

COMPONENTS PROVIDED

Description	Code	Quantity
Pancreatic Derived Factor/FAM3B Microplate - 96 well polystyrene microplate (12 strips of 8 wells) coated with an antibody against human Pancreatic Derived Factor/FAM3B.	344-01-01	1 plate
Pancreatic Derived Factor/FAM3B Standard – 200 ng/vial of recombinant human Pancreatic Derived Factor/FAM3B in a buffered protein base with preservative; lyophilized.	344-01-02	1 vial
Detection Antibody-Biotinylated – 105 µL/vial of 100-fold concentrated solution of antibody biotinylated against human Pancreatic Derived Factor/FAM3B.	344-01-03	1 vial
Positive Control – one vial of recombinant human Pancreatic Derived Factor/FAM3B; lyophilized.	344-01-04	1 vial
Streptavidin HRP Conjugate – 120 µL/vial of 100-fold concentrated solution of Streptavidin HRP conjugate	SAHRP	1 vial
Dilution Buffer – 60 mL of buffered protein based solution with preservative.	DB06	1 bottle
Antibody Diluent Solution– 12 mL of buffered protein based solution with preservative.	DB08	1 bottle
Wash Buffer - 50 mL of 10-fold concentrated buffered surfactant, with preservative.	WB01	1 bottle

Substrate Solution - 11 mL of substrate solution.	SS01	1 bottle
Stop Solution - 11 mL of 0.5M HCl.	S-STOP	1 bottle
Plate Sealer	EAPS	1
Plastic Pouch	P01	1

STORAGE

Unopened Kit: Store at 2 – 8° C for up to 6 months. For longer storage, unopened Standard, Positive Control and Detection Antibody-HRP Conjugate 100-fold concentrated solution should be stored at -20° C or -70° C. Substrate Solution can be stored at 2 – 8° C for up to 6 months (**DO NOT FREEZE** and **PROTECT FROM LIGHT**). All other components can be stored at 2 – 8° C for up to 6 months. Do not use kit past expiration date.

Opened / Reconstituted Reagents: Reconstituted Standard (stock) solution SHOULD BE STORED at -20° C or -70° C for up to one month.

Microplate Wells: Return unused microplate strips to the plastic pouch with the desiccant pack. Microplate may be stored for up to 6 months at 2 – 8° C.

ADDITIONAL MATERIALS REQUIRED

- Microplate reader capable of absorbance measurement at 450 nm.
- Microplate shaker (250 – 300 rpm).
- Microplate washer or manifold dispenser.
- 100 mL and 500 mL graduated cylinders.
- Multi-channel Pipette, Pipettes and pipette tips.
- Deionized or distilled water.

PRECAUTION

This kit should be handled by those persons who have been trained in and can follow the principles of good laboratory practice. Wear protective clothing such as laboratory overalls, safety glasses and gloves. Care should be taken while handling solutions in this kit to avoid contact with skin or eyes, especially with the stop solution because it contains diluted hydrochloric acid. Wash immediately with water in case of contact on skin or eyes.

SAMPLE COLLECTION AND STORAGE

Cell Culture Supernates - Remove particulates by centrifugation and assay immediately or aliquot and store samples at ≤-20 °C. Avoid repeated freeze-thaw cycles.

Serum - Use a serum separator tube (SST) and allow samples to clot for 30 minutes before centrifugation for 15 minutes at 1000 x g. Remove serum and assay immediately or aliquot and store samples at ≤ -20 °C. Avoid repeated freeze-thaw cycles.

Plasma - Collect plasma using EDTA, heparin, or citrate as an anticoagulant. Centrifuge for 15 minutes at 1000 x g within 30 minutes of collection. Assay immediately or aliquot and store samples at ≤ -20 °C. Avoid repeated freeze-thaw cycles.

Optional: Use Aprotinin (enzyme inhibitor) for ALL sample collection to prevent sample degradation. 0.5 TIU per ml of sample solution.

SAMPLE PREPARATION

Optimal dilutions should be determined by each laboratory for each application. Use polypropylene test tubes.


REAGENT PREPARATION

Bring all reagents to room temperature before use.

Wash Buffer - If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved. Dilute 50 mL of Wash Buffer Concentrate into deionized or distilled water (450 mL) to prepare 500 mL of 1x Wash Buffer.

FAM3B Standard - Reconstitute the FAM3B Standard with 1.0 mL of Dilution Buffer. This reconstitution produces a stock solution of 200 ng/mL. Allow the stock standard to sit for at least 15 minutes with gentle agitation until completely dissolved prior to making standard dilutions (see below). Mix each tube thoroughly before the next transfer. The **200 ng/mL** standard serves as the high standard. The Dilution Buffer serves as the zero standard (0 ng/mL).

Tube	Standard	Dilution Buffer	Concentration
Stock	Powder	1000 µl	200 ng/ml
# 1	250 µl of stock	250 µl	100 ng/ml
# 2	250 µl of 1	250 µl	50 ng/ml
# 3	250 µl of 2	250 µl	25 ng/ml
# 4	250 µl of 3	250 µl	12.5 ng/ml
# 5	250 µl of 4	250 µl	6.25 ng/ml

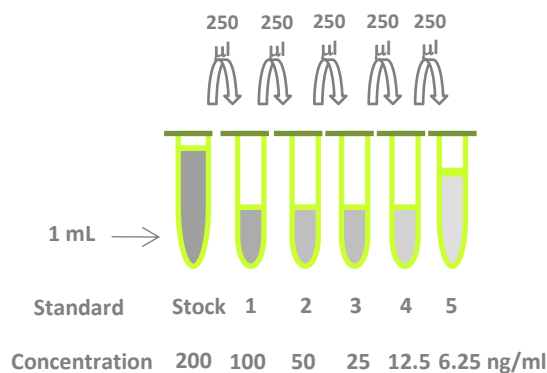

Positive Control - Reconstitute the Positive Control with 1.0 mL of Dilution Buffer. **NOTE:** Positive control could be reused within a few days if stored at $-20\text{ }^{\circ}\text{C} \sim -70\text{ }^{\circ}\text{C}$.

Detection Antibody - Reconstitute the Detection Antibody Concentrate with 1.05 mL of **Antibody Diluent Solution (DB08)** to produce a 10-fold concentrated stock solution. Pipette 9.45 mL of Antibody Diluent Solution (DB08) into a 15 mL centrifuge tube and transfer 1.05 mL of 10-fold concentrated stock solution to prepare working solution.

Streptavidin-HRP Conjugate - Transfer 120 μL of 100-fold concentrated Streptavidin-HRP conjugate stock solution to 11.88 mL of **HRP Diluent Solution (DB06)** to prepare working solution. **Note:** 1x working solution of Streptavidin-HRP Conjugate should be used within a few days (**protect from light**).

ELISA PROTOCOL

Bring all reagents and samples to room temperature before the start of the assay. Blank, standard dilutions, positive control and samples should be assayed in duplicate. ELISA Protocol may need further optimization.

1. Prepare all reagents and working standards as directed in the previous sections.
2. Remove excess microplate strips from the plate frame, return them to the plastic pouch with the desiccant pack.
3. Add 100 μL of Dilution Buffer to Blank wells.

4. Add 100 μL of Standard dilutions, sample, or positive control per well. Cover with plate sealer. Incubate for 2 hours on microplate shaker at room temperature.
5. Aspirate each well and wash, repeating the process three times for a total of four washes. Wash by filling each well with 1x Wash Buffer (300 μL) using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.
6. Add 100 μL of 1x Detection Antibody working solution to each well. Cover with plate sealer. Incubate for 2 hour on microplate shaker at room temperature.
7. Repeat the aspiration/wash as in step 5.
8. Add 100 μL of **Streptavidin-HRP Conjugate working solution** to each well. Incubate for 45 minutes on microplate shaker at room temperature. **Protect from light.**
9. Repeat the aspiration/wash as in step 5
10. Add 100 μL of Substrate Solution to each well. Incubate for 8-12 minutes on microplate shaker at room temperature. **Protect from light.**
11. Add 100 μL of Stop Solution to each well. The color in the wells should change from blue to yellow. If the color in the wells is green, or if the color change does not appear uniform, gently tap the plate to ensure thorough mixing.
12. Determine the optical density of each well within 15 minutes, using a microplate reader set to 450 nm.

CALCULATION OF RESULTS

Create a standard curve by plotting the log of the known concentrations of the standard dilutions (x-axis) versus the log of its corresponding O.D. (y-axis) and draw the best fit line through the points. It is recommended to use computer software capable of generating a four parameter logistic (4-pl) curve fit to more accurately quantify the standard dilutions.

If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

TYPICAL DATA

This standard curve is provided for demonstration only. A new standard curve should be generated for each set of samples assayed.

STANDARD (NG/ML)	AVERAGE OD450 (CORRECTED)
Blank	0 (0.079)
6.25	0.008
12.5	0.043
25	0.147
50	0.351
100	0.619
200	0.815

SPECIFICITY

PROTEINS	CROSS-REACTIVITY
Human FAM3B	100
Human Insulin	0
Human REG-1alpha	0

LINEARITY

To assess the linearity of the assay pooled research human **serum** samples were diluted with Dilution Buffer (DB08) and assayed.

DILUTION FACTOR	ASSAYED (NG/ML)	FINAL (NG/ML)	RECOVERY (%)
1 X	10.135	10.135	100
2 X	5.174	10.348	102
4 X	2.940	11.760	116

To assess the linearity of the assay pooled research human **EDTA plasma** samples were diluted with Dilution Buffer (DB08) and assayed.

DILUTION FACTOR	ASSAYED (NG/ML)	FINAL (NG/ML)	RECOVERY (%)
1 X	11.498	11.498	100
2 X	6.019	12.039	105
4 X	3.073	12.292	107

SUMMARY OF ASSAY PROCEDURE

