

HUMAN FIBROBLAST GROWTH FACOTR ACIDIC (FGF ACIDIC) ELISA KIT

FOR THE QUANTITATIVE DETERMINATION
OF HUMAN FGF ACIDIC CONCENTRATIONS
IN CELL CULTURE SUPERNATES, SERUM,
AND PLASMA



ALWAYS REFER TO LOT SPECIFIC PROTOCOL
PROVIDED WITH EACH KIT FOR
INSTRUCTIONS. PROTOCOL MUST BE
READ BEFORE USING THIS PRODUCT.

FOR RESEARCH USE ONLY. NOT FOR USE IN
DIAGNOSTIC PROCEDURES.

PRODUCT INFORMATION:

| ELISA NAME | HUMAN FGF ACIDIC ELISA KIT |
|--------------------------|---|
| Catalog No. | SK00354-01 |
| Lot No. | |
| Formulation | 96 T |
| Standard range | 78 – 5000 pg/mL |
| Sensitivity | 10 pg/mL |
| Sample Volume | 100 µl |
| Dilution Factor | Optimal dilutions should be determined by each laboratory for each application |
| Sample Type | Serum, EDTA Plasma, Cell Culture Supernates |
| Specificity | Human FGF Acidic |
| Calibration | FGF Acidic (FGF-1) |
| Intra-assay Precision | 4-6% |
| Inter-assay Precision | 8-10% |
| Storage | 2-8°C |

Order Contact:
AVISCERA BIOSCIENCE, INC.
2348 Walsh Ave., Suite C
Santa Clara, CA 95051
USA
Tel: (408) 982 0300
Fax: (408) 982 0301
Email: Sales@AvisceraBioscience.com
Info@AvisceraBioscience.com
www.AvisceraBioscience.com

DESCRIPTION

This Human FGF Acidic ELISA Kit contains the necessary components required for the quantitative measurement of recombinant and/or natural FGF1 from cell culture supernates, serum and plasma in a sandwich ELISA format.

This immunoassay contains recombinant human FGF Acidic and antibodies raised against this protein. Results from this immunoassay have shown to accurately quantify recombinant and natural FGF1 samples.

ASSAY OVERVIEW

This assay employs the quantitative sandwich ELISA format. The plate is pre-coated with a monoclonal antibody specific for FGF acidic. The capture antibody can bind to the FGF acidic in the standard and samples. After washing the plate of any unbound substances, a biotinylated monoclonal antibody against human FGF acidic is added to the wells. After another washing of the plate, Streptavidin-HRP Conjugate is added. After the last wash to remove any unbound enzyme, a substrate solution (TMB) is added to the wells and color develops in direct proportion to the amount of FGF acidic bound in the standard solutions or samples. A standard curve can be established and sample values can be read off the standard curve.

PROCEDURAL LIMITATIONS

_FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

_This ELISA kit should not be used beyond the expiration date on the kit label.

_Do not mix reagents with those from other lots or sources.

_It is important that the Dilution Buffer selected for the standard curve be consistent with the samples being assayed.

_Each laboratory must determine the optimal dilution factors for the samples being assayed with a pretest. If samples generate values that are not within the dynamic range of the standard curve, further concentrate or dilute the samples as required with Dilution Buffer and repeat the assay.

_Any modifications in buffers, pipetting technique, washing technique, incubation time or temperature, as well as kit age can cause a change in signal.

_Not all interfering factors have been tested in the immunoassay, therefore the possibility of interference cannot be excluded.

COMPONENTS PROVIDED

| DESCRIPTION | CODE | QUANTITY |
|--|------------------|-----------------|
| FGF acidic Microplate - 96 well polystyrene microplate (12 strips of 8 wells) coated with a monoclonal antibody against human FGF acidic | 354-01-01 | 1 plate |
| Human FGF acidic Standard – 10 ng/vial of recombinant human FGF acidic in a buffered protein base with preservative; lyophilized. | 354-01-02 | 1 vial |
| Detection Antibody – 1.2 mL/vial, 10-fold concentrate of biotinylated purified monoclonal antibody against human FGF acidic with preservative; lyophilized. | 354-01-03 | 1 vial |
| Positive Control – one vial of recombinant human FGF acidic; lyophilized. | 354-01-04 | 1 vial |
| Streptavidin-HRP Conjugate - 120 µL/vial, 100-fold concentrated solution of Streptavidin conjugate to HRP. | SAHRP | 1 vial |
| Dilution Buffer – 60 mL of buffered protein based solution with preservative. | DB09 | 1 bottle |
| Antibody & HRP Diluent Solution – 30 mL of buffered protein based solution with preservative. | DB08 | 1 bottle |
| Wash Buffer - 50 mL of 10-fold concentrated buffered surfactant, with preservative. | WB01 | 1 bottle |
| TMB Substrate Solution - 11 mL of TMB substrate solution. | TMB01 | 1 bottle |
| Stop Solution – 11 mL of 0.5M HCl. | S-STOP | 1 bottle |
| Plate Sealer | EAPS | 1 piece |
| Plastic Pouch | P01 | 1 piece |

STORAGE

Unopened Kit: Store at 2 - 8° C for up to 8 months. For longer storage, unopened Standard, Positive Control and Detection Antibody Concentrate should be stored at -20 or -70°C. Do not use kit past expiration date.

Opened / Reconstituted Reagents: Reconstituted Standard and Detection Antibody Concentrate Solution SHOULD BE STORED at -20°C or -70°C for up to one month. Streptavidin-HRP Conjugate 100-fold concentrated solution and TMB Substrate Solution can be stored at 2 – 8 °C for up to 8 months (**DO NOT FREEZE** and **PROTECT FROM LIGHT**). All other components may be stored at 2 – 8 °C for up to 8 months.

Microplate Wells: Return unused wells to the plastic pouch with the desiccant pack. Microplate may be stored for up to 6 months at 2 - 8°C after opening.

PRECAUTION

This kit should be handled by those persons who have been trained in and can follow the principles of good laboratory practice. Wear protective clothing such as laboratory overalls, safety glasses and gloves. Care should be taken while handling solutions in this kit to avoid contact with skin or eyes, especially with the stop solution because it contains diluted hydrochloric acid. Wash immediately with water in case of contact on skin or eyes.

ADDITIONAL MATERIALS REQUIRED

- Microplate reader capable of absorbance measurement at 450 nm.
- Microplate shaker (250 – 300 rpm).
- Microplate washer or manifold dispenser.
- 100 mL and 500 mL graduated cylinders.
- Multi-channel Pipette, Pipettes and pipette tips.
- Deionized or distilled water.

SAMPLE COLLECTION AND STORAGE

Cell Culture Supernates - Remove particulates by centrifugation and assay immediately or aliquot and store samples at ≤-20° C. Avoid repeated freeze-thaw cycles. *Try to use animal free media.*

Serum - Use a serum separator tube (SST) and allow samples to clot for 30 minutes before centrifugation for 15 minutes at 1000 x g. Remove serum and assay immediately or aliquot and store samples at ≤ -20° C. Avoid repeated freeze-thaw cycles.

Plasma - Collect plasma using EDTA, heparin, or citrate as an anticoagulant. Centrifuge for

15 minutes at 1000 x g within 30 minutes of collection. Assay immediately or aliquot and store samples at ≤-20° C. Avoid repeated freeze-thaw cycles.

Optional: Use Aprotinin (enzyme inhibitor) for ALL sample collection to prevent sample degradation. 0.5 TIU per ml of sample solution.

SAMPLE PREPARATION

Serum and plasma samples may not require dilution. If the samples levels are over 5 ng/ml, may require a 2-fold dilution. A suggested 2-fold dilution is 125 µL sample + 125 µL Dilution Buffer. **Optimal dilutions should be determined by each laboratory for each application with a sample pretest.**

Use polypropylene test tubes.


REAGENT PREPARATION

Bring all reagents to room temperature before use.

Wash Buffer - If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved. Dilute 50 mL of Wash Buffer Concentrate into deionized or distilled water (450 mL) to prepare 500 mL of 1x Wash Buffer.

Human FGF acidic Standard - Reconstitute the human FGF acidic Standard with 1 ml of Dilution Buffer. This reconstitution produces a stock solution of 10 ng/mL. Allow the standard to sit for a minimum of 15 minutes with gentle agitation prior to making dilutions. Pipette 250 µL of Dilution Buffer into tubes #1 to #7. Use the stock solution to produce a dilution series (below). Mix each tube thoroughly before the next transfer. The 5 ng/mL standard serves as the high standard. The Dilution Buffer serves as the zero standard (0 ng/mL).

| TUBE | STANDARD | DILUTION BUFFER | CONCENTRATION |
|-------|----------------|-----------------|---------------|
| stock | powder | 1 ml | 10 ng/ml |
| # 1 | 250µl of stock | 250µl | 5 ng/ml |
| # 2 | 250µl of 1 | 250µl | 2.5 ng/ml |
| # 3 | 250µl of 2 | 250µl | 1.25 ng/ml |
| # 4 | 250µl of 3 | 250µl | 0.625 ng/ml |
| # 5 | 250µl of 4 | 250µl | 0.3125 ng/ml |
| # 6 | 250µl of 5 | 250µl | 0.156 ng/ml |
| # 7 | 250µl of 6 | 250µl | 0.078 ng/ml |

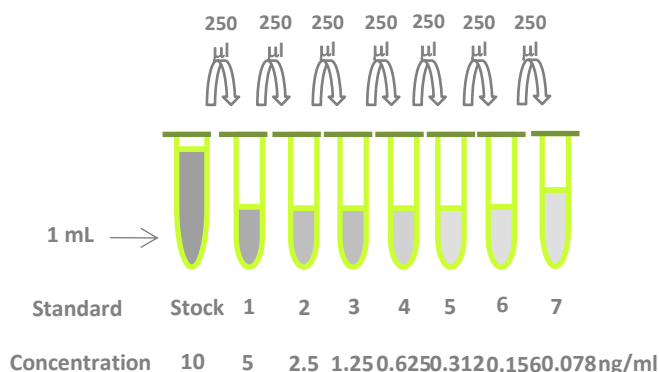

Detection Antibody - Reconstitute the Detection Antibody Concentrate with 1.2 mL of Antibody & HRP Diluent Solution (**DB08**) to produce a 10-fold concentrated stock solution. Pipette 10.8 mL of Dilution Buffer into a 15 mL centrifuge tube and transfer 1.2 mL of 10-fold concentrated stock solution to prepare working solution.

Streptavidin-HRP Conjugate - Pipette 11.88 mL of Antibody & HRP Diluent Solution (**DB08**) into a 15 mL centrifuge tube and transfer 120 µL of 100-fold concentrated stock solution to prepare working solution. *Note: 1x working solution of Streptavidin-HRP Conjugate should be used within a few days (protect from light).*

Positive Control - Reconstitute the Positive Control with 1.0 mL of Dilution Buffer. Note: Positive Control could be used within a few days if stored at -20 °C or -70 °C.

ELISA PROTOCOL

Bring all reagents and samples to room temperature before the start of the assay. Blank, standard dilutions, positive control and samples should be assayed in duplicate. ELISA Protocol may need further optimization.


1. Prepare all reagents and working standards as directed in the previous sections.
2. Remove excess microplate strips from the plate frame, return them to the plastic pouch with the desiccant pack and seal.
3. Add 100 µL per well of Dilution Buffer to Blank wells.

4. Add 100 µL of Standard, sample, or positive control per well. Cover with plate sealer. Incubate for 2 hours on microplate shaker at room temperature.
5. Aspirate each well and wash, repeating the process three times for a total of four washes. Wash by filling each well with 1x Wash Buffer (300 µL) using a squirt bottle, manifold dispenser, or autowasher. Complete removal of liquid at each step is essential to good performance. After the last wash, remove any remaining Wash Buffer by aspirating or decanting. Invert the plate and blot it against clean paper towels.
6. Add 100 µL of Detection Antibody working solution to each well. Cover with plate sealer. Incubate for 2 hours on microplate shaker at room temperature.
7. Repeat the aspiration/wash as in step 5.
8. Add 100 µL of **Streptavidin-HRP Conjugate working solution** to each well. Incubate for 40 min on microplate shaker at room temperature. **Protect from light.**
9. Repeat the aspiration/wash as in step 5.
10. Add 100 µL of Substrate Solution to each well. Incubate for 20-25 minutes on microplate shaker at room temperature. **Protect from light.**
11. Add 100 µL of Stop Solution to each well. The color in the wells should change from blue to yellow. If the color in the wells is green, or if the color change does not appear uniform, gently tap the plate to ensure thorough mixing.
12. Determine the optical density of each well within 15 minutes, using a microplate reader set to 450 nm.

CALCULATION OF RESULTS

Create a standard curve by plotting the log of the known concentrations of the standard dilutions (x-axis) versus the log of its corresponding O.D. (y-axis) and draw the best fit line through the points. It is recommended to use computer software capable of generating a log-log curve fit to more accurately quantify the standard dilutions.

If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

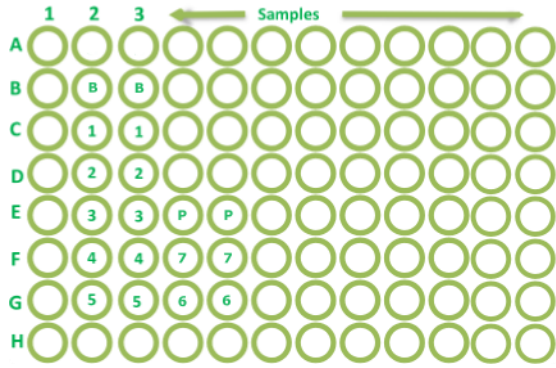

TYPICAL DATA

This standard curve is provided for demonstration only. A new standard curve should be generated for each set of samples assayed.

| STANDARD (PG/ML) | AVERAGE OD450NM (CORRECTED) |
|------------------|-----------------------------|
| Blank | 0 (0.049) |
| 78 | 0.016 |
| 156 | 0.048 |
| 312.5 | 0.119 |
| 625 | 0.291 |
| 1250 | 0.445 |
| 2500 | 0.622 |
| 5000 | 1.291 |

SPECIFICITY

| PROTEINS | CROSS-REACTIVITY (%) |
|------------------|----------------------|
| Human FGF acidic | 100 |
| Human FGF-2 | 0 |
| Human FGF-19 | 0 |
| Human FGF-21 | 0 |
| Human FGF-23 | 0 |

LINEARITY

To assess the linearity of the assay, pooled research human serum and EDTA plasma samples were diluted with Dilution Buffer DB09 and assayed.

| SAMPLE TYPE | DILUTION FACTOR | ASSAYED (PG/ML) | FINAL (PG/ML) | RECOVERY (%) |
|--------------|-----------------|-----------------|---------------|--------------|
| HUMAN SERUM | 1 X | 289.971 | 289.971 | 100 |
| HUMAN SERUM | 2 X | 160.681 | 321.362 | 110.8 |
| HUMAN PLASMA | 1 X | 733.572 | 733.572 | 100 |
| HUMAN PLASMA | 2 X | 329.618 | 659.236 | 89.9 |

SUMMARY OF ASSAY PROCEDURE

PREPARE REAGENTS, SAMPLES AND STANDARDS

↓

Add 100 µL of standard, samples, positive control to each well. Incubate 2 hours on the plate shaker at RT.

↓

Aspirate and wash 4 times.

↓

Add 100 µL Detection Antibody working solution to each well. Incubate 2 hours on the plate shaker at RT.

↓

Aspirate and wash 4 times.

↓

Add 100 µL Streptavidin-HRP conjugate working solution to each well. Incubate 40 min on the plate shaker at RT. **Protect from light.**

↓

Aspirate and wash 4 times.

↓

Add 100 µL Substrate Solution to each well. Incubate 20-25 min on the plate shaker at RT. **Protect from light.**

↓

Add 100 µL Stop Solution to each well. Read 450nm within 15 min.