

HIGH SENSITIVITY PRO BRAIN-DERIVED NEUROTROPHIC FACTOR (PRO-BDNF) HUMAN ELISA KIT

FOR THE QUANTITATIVE DETERMINATION OF
HUMAN PRO-BDNF CONCENTRATIONS IN PLASMA
AND SERUM



ALWAYS REFER TO LOT SPECIFIC
PROTOCOL PROVIDED WITH EACH KIT FOR
INSTRUCTIONS. PROTOCOL MUST BE
READ AND CHECK ALL ITEMS OF EACH KIT
BEFORE USING THIS PRODUCT.

FOR RESEARCH USE ONLY. NOT FOR USE IN
DIAGNOSTIC PROCEDURES.

PRODUCT INFORMATION:

THIS KIT IS FOR ONE TIME USE ONLY.

ELISA Name	HIGH SENSITIVITY PRO-BDNF HUMAN ELISA KIT
Catalog No.	SK00752-05-HS
Lot No.	20115190
Formulation	96 T
Standard range	15.6 ~ 4000 pg/mL
Sensitivity	5 pg/mL
Sample Volume	100 µL
Dilution Factor	4 ~ 8 for Serum or Plasma
Sample Type	Serum, Plasma
Specificity	Human Pro-BDNF (19-247)
Calibration	Human Pro-BDNF (19-247) Recombinant (HEK293 derived)
Intra-assay Precision	4 - 6%
Inter-assay Precision	5 - 10%
Storage	2 – 8° C for 8 months, more information check page 2-3
This kit contains sufficient materials to run approximately 35~40 samples duplicated provided that assay is run according to protocol.	

ORDER CONTACT:

AVISCERA BIOSCIENCE, INC.

1289 HAMMERWOOD AVE SUITE-B,
SUNNYVALE CA94089, USA

Tel: (408) 982 0300

Email: Sales@AvisceraBioscience.com

www.AvisceraBioscience.com

www.AvisceraBioscience.net

DESCRIPTION

This High Sensitivity Pro-BDNF Human ELISA Kit contains the necessary components required for the quantitative measurement of recombinant human Pro BDNF (19- 247) (HEK293) and/or natural human Pro-BDNF (19-247) from plasma and serum samples in a sandwich ELISA format.

This immunoassay contains human Pro-BDNF (19-247) recombinant and antibodies raised against this protein. Results from this immunoassay have shown to accurately quantify bioactive recombinant and natural Pro-BDNF (19-247) in the samples. The mature form BDNF (129-247) or Pro BDNF (19-128) in the samples cannot be detected by this ELISA kit.

ASSAY OVERVIEW

This assay employs the quantitative sandwich ELISA format. The plate is pre-coated with a monoclonal antibody specific for human bioactive Pro-BDNF (19-247). The capture antibody can bind to the human bioactive Pro-BDNF in the standard and samples. After washing the plate of any unbound substances, a biotinylated monoclonal antibody against human Pro-BDNF (19-247) is added to the wells. After another washing of the plate, Streptavidin-HRP Conjugate is added. After the last wash to remove any unbound enzyme, a substrate solution (TMB) is added to the wells and color develops in direct proportion to the amount of human Pro-BDNF (19-247) bound in the standard solutions or samples. A standard curve can be established and sample values can be read off the standard curve.

PROCEDURAL LIMITATIONS

_FOR RESEARCH USE ONLY. NOT FOR USE IN DIAGNOSTIC PROCEDURES.

_This ELISA kit should not be used beyond the expiration date on the kit label.

_Do not mix reagents with those from other lots or sources.

_It is important that the Dilution Buffer selected for the standard curve be consistent with the samples being assayed.

_Each laboratory must determine the optimal dilution factors for the samples being assayed with a pretest.

_Any modifications in buffers, pipetting technique, washing technique, incubation time or temperature, as well as kit age can cause a change in signal.

_Not all interfering factors have been tested in the immunoassay, therefore the possibility of interference cannot be excluded.

COMPONENTS PROVIDED

DESCRIPTION	CODE	QUANTITY
Pro-BDNF Microplate - 96 well polystyrene microplate (12 strips of 8 wells) coated with a monoclonal antibody against Pro-BDNF.	752-05-HS-01	1 plate
Pro-BDNF Standard – 16 ng/vial of recombinant human Pro-BDNF in a buffered protein base with preservative; lyophilized.	752-05-HS-02	1 vial
Detection Antibody Concentrate – 1.2 mL/vial of 10-fold concentrate of biotinylated antibody against Pro-BDNF with preservative; lyophilized.	752-05-HS-03	1 vial
Positive Control - one vial of recombinant human Pro-BDNF; lyophilized.	752-05-HS-04	1 vial
Streptavidin-HRP Conjugate – 120 µL/vial, 100-fold concentrated solution of Streptavidin conjugate to HRP.	SAHRP	1 vial
Dilution Buffer - 45 mL of buffered solution with preservative.	DB90	1 bottle
HRP Diluent Solution - 12 mL of buffered protein based solution with preservative.	DB08C	1 bottle
Wash Buffer 20X - 25 mL of 20-fold concentrated buffered surfactant, with preservative.	WB01	1 bottle
TMB Substrate Solution - 11 mL of TMB substrate solution.	TMB01	1 bottle
Stop Solution - 11 mL of 0.125M HCl solution.	S-STOP	1 bottle
Plate Sealer	EAPS	1
Plastic Pouch	P01	1

STORAGE

Unopened Kit: Store at 2 – 8° C up to 8 months. For longer storage up to 12 months, unopened Standard, Positive Control, Detection Antibody Concentrate, Dilution Buffer and HRP Diluent Solution should be stored at -20° C.

Streptavidin-HRP Conjugate and TMB Substrate Solution should be stored only at 2 ~ 8°C.

Do not use kit past expiration date.

ADDITIONAL MATERIALS REQUIRED

- Microplate reader capable of absorbance measurement at 450 nm.
- Microplate shaker (250 – 300 rpm).
- Microplate washer or manifold dispenser.
- 100 mL and 500 mL graduated cylinders.
- Multi-channel Pipette, Pipettes and pipette tips.
- Deionized or distilled water.

PRECAUTION

This kit should be handled by those persons who have been trained in and can follow the principles of good laboratory practice. Wear protective clothing such as laboratory overalls, safety glasses and gloves. Care should be taken while handling solutions in this kit to avoid contact with skin or eyes, especially with the stop solution because it contains diluted hydrochloric acid. Wash immediately with water in case of contact on skin or eyes.

SAMPLE COLLECTION AND STORAGE

Serum - Use a serum separator tube (SST) and allow samples to clot for 30 minutes before centrifugation for 15 minutes at 1000 x g. Remove serum and assay immediately or aliquot and store samples at ≤ -20° C. Avoid repeated freeze-thaw cycles.

Plasma - Collect plasma using EDTA, heparin, or citrate as an anticoagulant. Centrifuge for 15 minutes at 1000 x g within 30 minutes of collection. Assay immediately or aliquot and store samples at ≤ -20° C. Avoid repeated freeze-thaw cycles.

Optional: Use Aprotinin (enzyme inhibitor) for ALL sample collection to prevent sample degradation. 0.5 TIU per ml of sample solution.

SAMPLE PREPARATION

Plasma or serum samples may need 4~8 fold dilution for best sample recovery.

A suggested 4-fold dilution is 25 µl per well of sample + 75 µl per well of Dilution Buffer DB90. A suggested 8-fold dilution is 12.5 µl per well of sample + 87.5 µl per well of Dilution Buffer DB90.

Optimal dilutions should be determined by each laboratory for each application with a pretest. Use polypropylene test tubes.

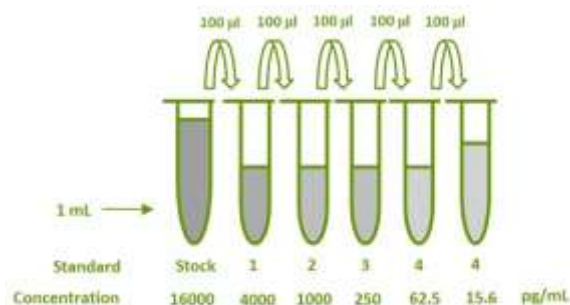
REAGENT PREPARATION

Bring all reagents to room temperature before use.

Wash Buffer - If crystals have formed in the concentrate, warm to room temperature and mix gently until the crystals have completely dissolved. Dilute **25 mL** of Wash Buffer Concentrate into deionized or distilled water (**475 mL**) to prepare 500 mL of 1x Wash Buffer.

Pro-BDNF Standard - Reconstitute the Pro-BDNF standard with 1.0 mL of **Dilution Buffer DB90**. This reconstitution produces a stock solution of 16 ng/mL. Allow the standard to sit for a minimum of 5 minutes with gentle agitation prior to making dilutions. Use the stock solution to produce a dilution series (below). Mix each tube thoroughly before the next transfer. The **4000 pg/mL** standard serves as the high standard. The Dilution Buffer serves as the zero standard (0 pg/mL). Store the stock solution at -70 °C for a few days.

TUBE	STANDARD	DILUTION BUFFER	CONCENTRATION
stock	powder	1.0ml	16 ng/ml
# 1	100 µl of stock	300 µl	4000 pg/ml
# 2	100 µl of 1	300 µl	1000 pg/ml
# 3	100 µl of 2	300 µl	250 pg/ml
# 4	100 µl of 3	300 µl	62.5 pg/ml
# 5	100 µl of 4	300 µl	15.6 pg/ml



Positive Control - Reconstitute the Positive Control with 1 mL of Dilution Buffer to prepare 20 fold concentrated stock solution. Pipette 0.475 mL of **Dilution Buffer DB90** into a 1.5 mL vial and transfer 25 µL of 20 - fold concentrated stock solution to prepare working solution. Discard the positive control after use. It is for one time use only.

Detection Antibody - Reconstitute the Detection Antibody Concentrate with 1.2 mL of **Dilution Buffer DB90** to produce a 10-fold concentrated stock solution. For 96 wells test, freshly Pipette 9.45 mL of **Dilution Buffer DB90** into a 15 mL centrifuge tube and transfer 1.05 mL of 10-fold concentrated stock solution to prepare working solution. For the partial strip test, freshly prepare 900 µL per strip of working solution. Store the stock solution at -20 °C for a few days.

Streptavidin-HRP Conjugate - For 96 wells test, freshly Pipette 10.89 mL of **HRP Diluent Solution (DB08C)** into a 15 mL centrifuge tube and transfer 110 µL of 100-fold concentrated stock solution to prepare working solution (**protect from light**). The working solution of Streptavidin-HRP Conjugate should be freshly prepared and used within 10 min. For the partial strip test, freshly prepare 900 µL per strip of working solution. Store the stock solution at 2 ~ 8 °C for 12 months.

The Pro BDNF Microplate require pre-wash 3 times by filling each well with 1x Wash Buffer (300 µL) prior to perform Assay

ELISA PROTOCOL

Bring all reagents and samples to room temperature before the start of the assay. Blank, standard dilutions, positive control and samples should be assayed in duplicate. ELISA Protocol may need further optimization.

1. Prepare all reagents and working standards as directed in the previous sections.
2. Add 100 µL per well of Dilution Buffer to Blank wells.
3. Add 100 µL of standard dilutions, positive control, or samples per well. Cover with the plate sealer. Incubate for **2 hours** on microplate shaker at room temperature.

4. Discard the solution of each well by hold the edge of plate and quickly invert plate top down. Discard and wash, repeating the process three times for a total of four washes. Wash by filling each well with 1x Wash Buffer (300 µL) using a 8- channel pipette, or autowasher. Complete removal of liquid at each step is essential to good performance.
5. Add 100 µL of Detection Antibody working solution to each well. Cover with the plate sealer. Incubate for **90 minutes** on microplate shaker at room temperature.
6. Repeat the discard/wash as in step 4.
7. Add 100 µL of Streptavidin-HRP Conjugate working solution to each well. Incubate for **45 minutes** on microplate shaker at room temperature. **Protect from light.**
8. Repeat the discard/wash as in step 4.
9. Add 100 µL of Substrate Solution to each well. Incubate for 12 ~ 16 minutes on microplate shaker at room temperature. **Protect from light.**
10. Add 100 µL of Stop Solution to each well. The color in the wells should change from blue to yellow. If the color in the wells is green, or if the color change does not appear uniform, gently tap the plate to ensure thorough mixing.
11. Determine the optical density of each well using a microplate reader set to 450 nm within 5 min.

CALCULATION OF RESULTS

Create a standard curve by plotting the log of the known concentrations of the standard dilutions (x-axis) versus the log of its corresponding O.D. (y-axis) and draw the best fit line through the points. It is recommended to use computer software capable of generating a log-log or 4-Parameter curve fit to more accurately quantify the standard dilutions.

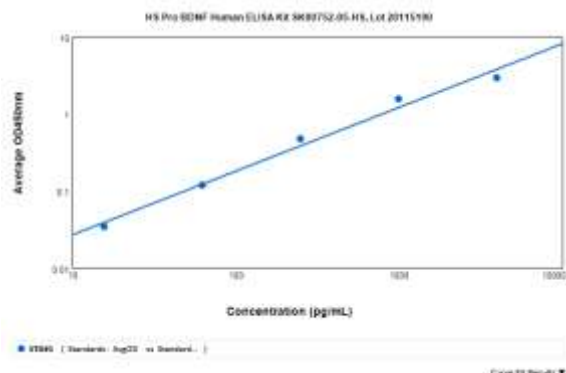
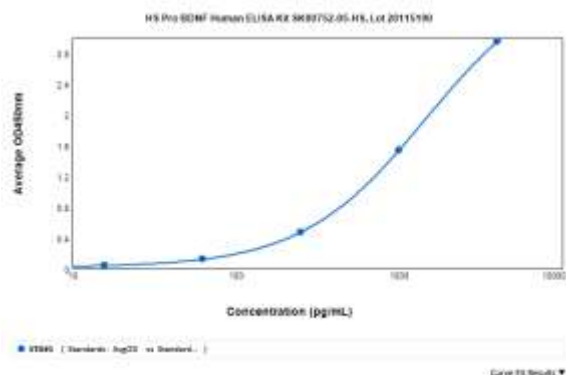
If samples have been diluted, the concentration read from the standard curve must be multiplied by the dilution factor.

TYPICAL STANDARD CURVE

This standard curve is provided for demonstration only. A new standard curve should be generated for each set of samples assayed.

STANDARD (PG/ML)	AVERAGE OD450NM (CORRECTED)
Blank	0 (0.129)
15.6	0.034
62.5	0.119
250	0.471
1000	1.540
4000	2.953

- Lot No.: 20115190
- Positive Control: 1x: 400 ~ 1600 pg/mL (log-log)

Standard curve by log-log fit:**Standard curve by 4-parameter fit:****SPECIFICITY**

PROTEINS	CROSS-REACTIVITY (%)
Human Pro-BDNF (19-247), R127A, R128A, (HEK293 derived)	100
Mouse Pro-BDNF (19-249), R129A, R130A, (HEK293 derived)	100
Human Pro-BDNF (19-128) His Tag (E. Coli)	0
Human BDNF, (HEK293 derived)	0
Human BDNF (CHO derived)	0
Human BDNF (Dimer) (E. Coli)	0
Human CNTF	0
Human GDNF	0
Human Pro NGF	0
Human NGF	0
Human NT-3	0

The data indicated that human Pro- BDNF (19-247) (*E. Coli* derived) and Human Pro- BDNF (19-128) (*E. Coli* derived) do not have any cross-reactivity with this human pro BDNF ELISA kit.

The mouse EDTA plasma and Serum can not be detected by this ELISA Kit.

SUMMARY OF ASSAY PROCEDURE

PREPARE REAGENTS, SAMPLES AND STANDARDS
↓ Pre-wash the plate. Add 100 µl of standard dilutions, samples, or positive control to each well. Incubate 2 hours on the plate shaker at RT.
↓ Discard and wash 4 times.
↓ Add 100 µl Detection Antibody working solution to each well. Incubate 90 min on the plate shaker at RT.
↓ Discard and wash 4 times.
↓ Add 100 µl Streptavidin HRP conjugate working solution to each well. Incubate 45 min on the plate shaker at RT. Protect from light.
↓ Discard and wash 4 times.
↓ Add 100 µl Substrate Solution to each well. Incubate 12 ~ 16 min on the plate shaker at RT. Protect from light.
↓ Add 100 µl Stop Solution to each well. Read at 450 nm within 5 min.

Well Position



Aviscera Bioscience' New Biomarker ELISA Kits for Metabolism or Neuroscience Research Use Only.

Biomarker Name	Catalog No.
Raptin/RCN2 (Mouse, Rat) ELISA Kit	SK00168-12
Raptin/RCN2 (Human) ELISA Kit	SK00168-18

Feimin/C5ORF24 Human ELISA Kit	SK00001-06
Cholesin/C7ORF50 Human ELISA Kit	SK00027-09
Endotrophin ETP Human ELISA Kit	SK00009-08
Mouse BDNF ELISA Kit High Sensitivity	SK00752-03U
GDF15 Human ELISA kit	SK00108-06
Soluble CD209 ELISA Kit	SK00345-09
EPDR1 Human ELISA Kit	SK00023-06
FAM19A1/TAFA1 Human ELISA Kit	SK00419-06
Human Pro-BDNF (19-247) ELISA Kit	SK00752-09HS
Beta Amyloid 40 Human ELISA Kit	SK00755-06
Beta Amyloid 42 Human ELISA Kit	SK00756-06
Pro-NGF (19-121) Human ELISA Kit	SK00307-08
Pro-NGF Total Human ELISA Kit	SK00307-06
Soluble Insulin Receptor ELISA Kit	SK00413-06

More information:

www.AvisceraBioscience.net